

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122923\
 Data File : VU057365.D
 Acq On : 29 Dec 2023 12:20
 Operator : MD/SY
 Sample : 06021-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	109	rVB	117715	137709	15.89%	2.013%
2	1.914	185	194	209	rVB	100801	134648	15.53%	1.969%
3	2.560	384	395	412	rVB	178017	295791	34.13%	4.325%
4	3.177	577	587	599	rVB2	5095	9661	1.11%	0.141%
5	4.640	1030	1042	1089	rBV2	82525	335739	38.74%	4.909%
6	5.055	1155	1171	1197	rBV2	169555	389856	44.98%	5.700%
7	5.717	1357	1377	1410	rBV2	314639	834238	96.25%	12.197%
8	6.245	1526	1541	1565	rBV	281911	549945	63.45%	8.041%
9	6.685	1663	1678	1702	rBV	202768	402577	46.45%	5.886%
10	7.563	1939	1951	1966	rBV	94070	169271	19.53%	2.475%
11	7.894	2038	2054	2078	rBV	335832	601341	69.38%	8.792%
12	8.174	2129	2141	2165	rBV3	55864	101516	11.71%	1.484%
13	8.634	2272	2284	2316	rBV2	399097	866740	100.00%	12.673%
14	9.412	2512	2526	2549	rBV	401498	680041	78.46%	9.943%
15	10.749	2930	2942	2956	rBV	150580	243939	28.14%	3.567%
16	11.807	3259	3271	3291	rBV	338902	547716	63.19%	8.008%
17	12.187	3377	3389	3407	rBV	298609	504386	58.19%	7.375%
18	12.769	3562	3570	3579	rVB	5677	9017	1.04%	0.132%
19	16.881	4841	4849	4860	rBV5	17403	25310	2.92%	0.370%




Sum of corrected areas: 6839441

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122923\
Data File : VU057365.D
Acq On : 29 Dec 2023 12:20
Operator : MD/SY
Sample : 06021-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

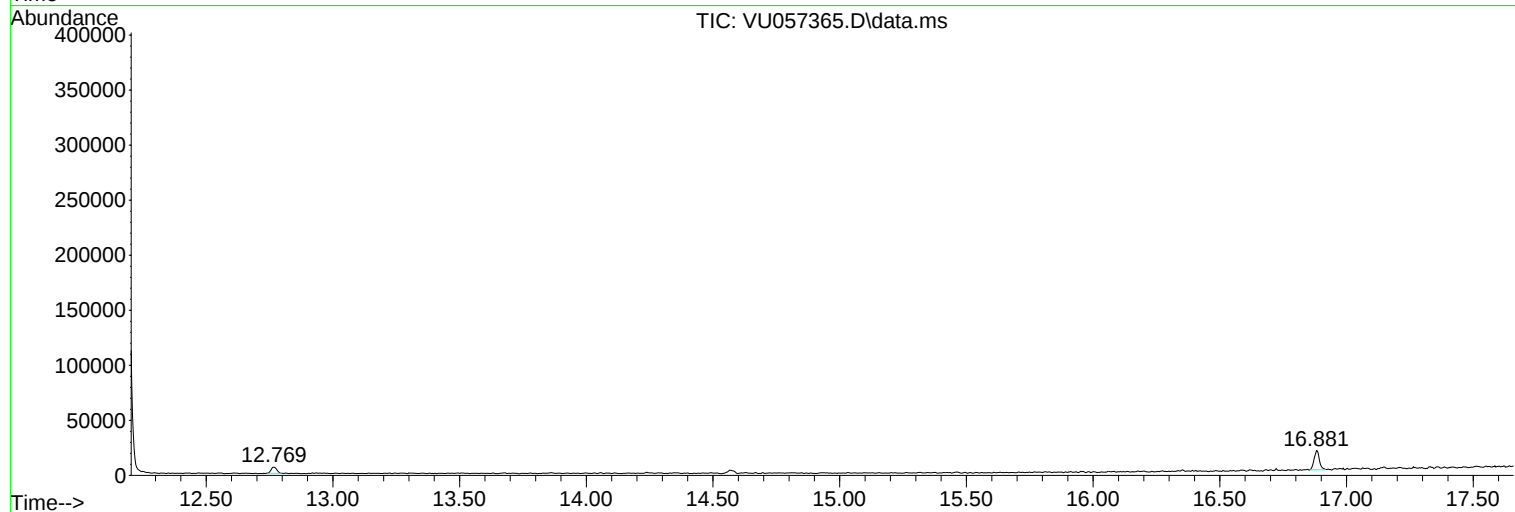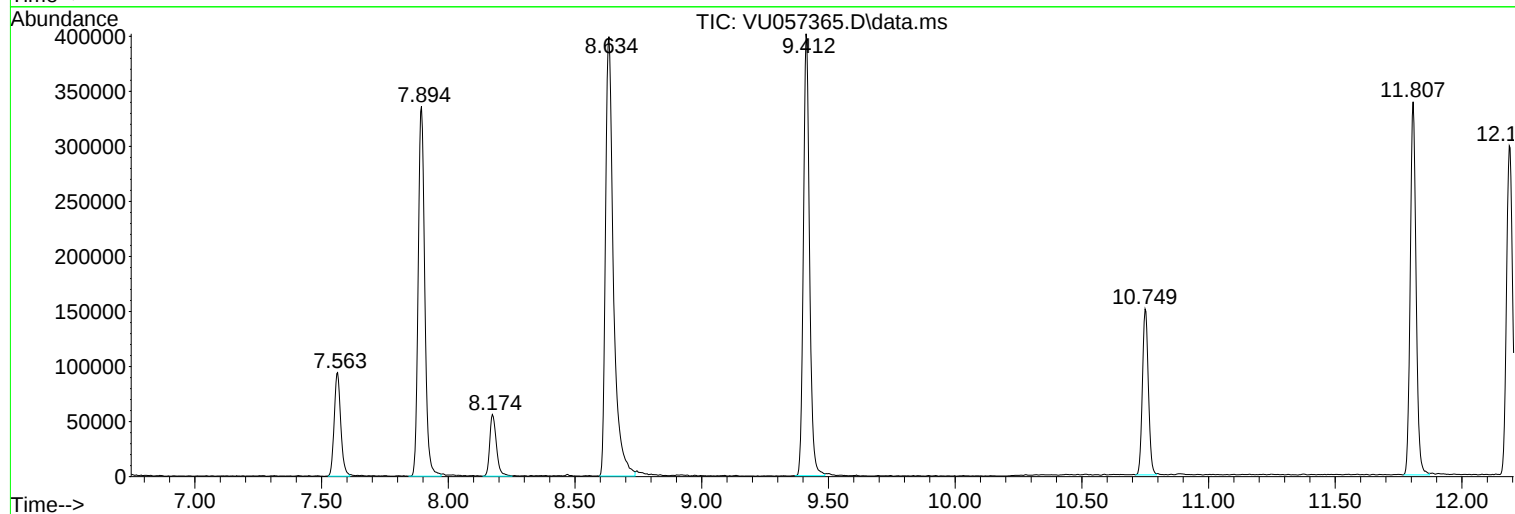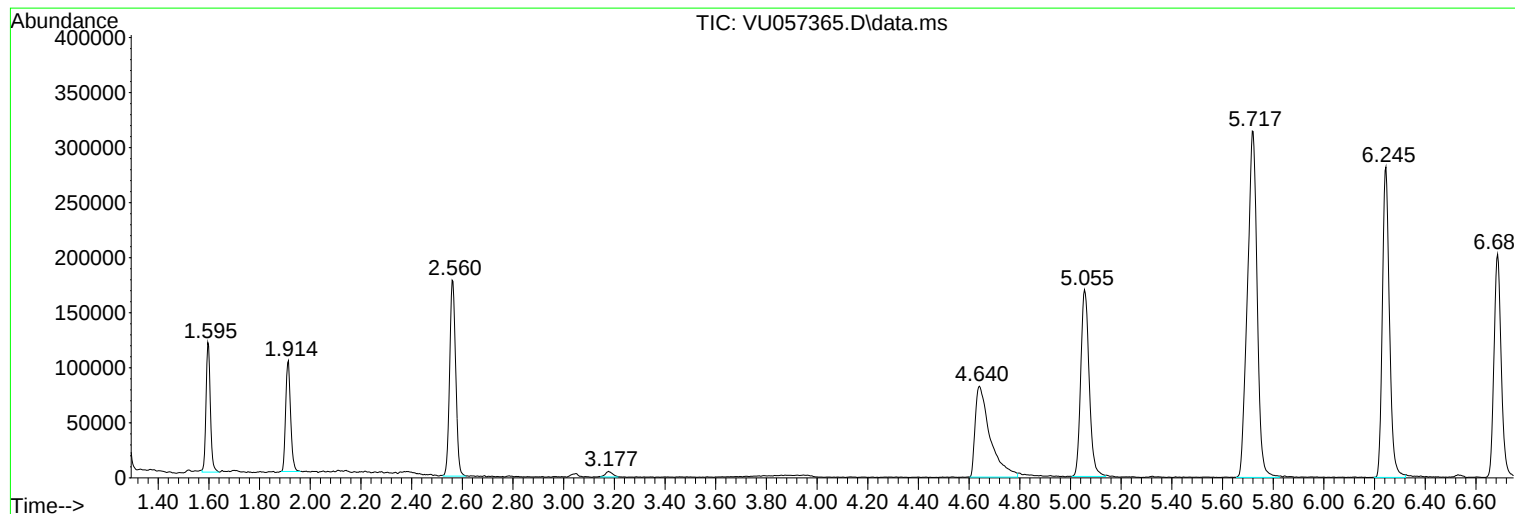

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122923\
Data File : VU057365.D
Acq On : 29 Dec 2023 12:20
Operator : MD/SY
Sample : 06021-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122923\
Data File : VU057365.D
Acq On : 29 Dec 2023 12:20
Operator : MD/SY
Sample : 06021-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc