
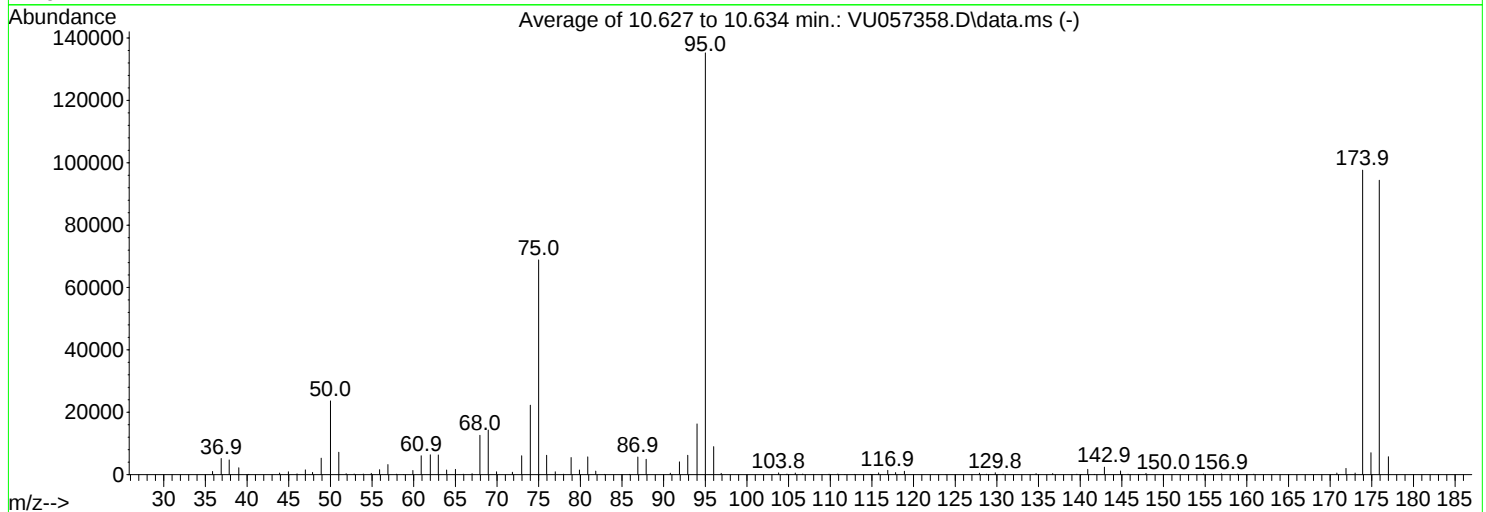


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122923\
Data File : VU057358.D
Acq On : 29 Dec 2023 08:51
Operator : MD/SY
Sample : BFB104
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB104

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 29 23:01:57 2023

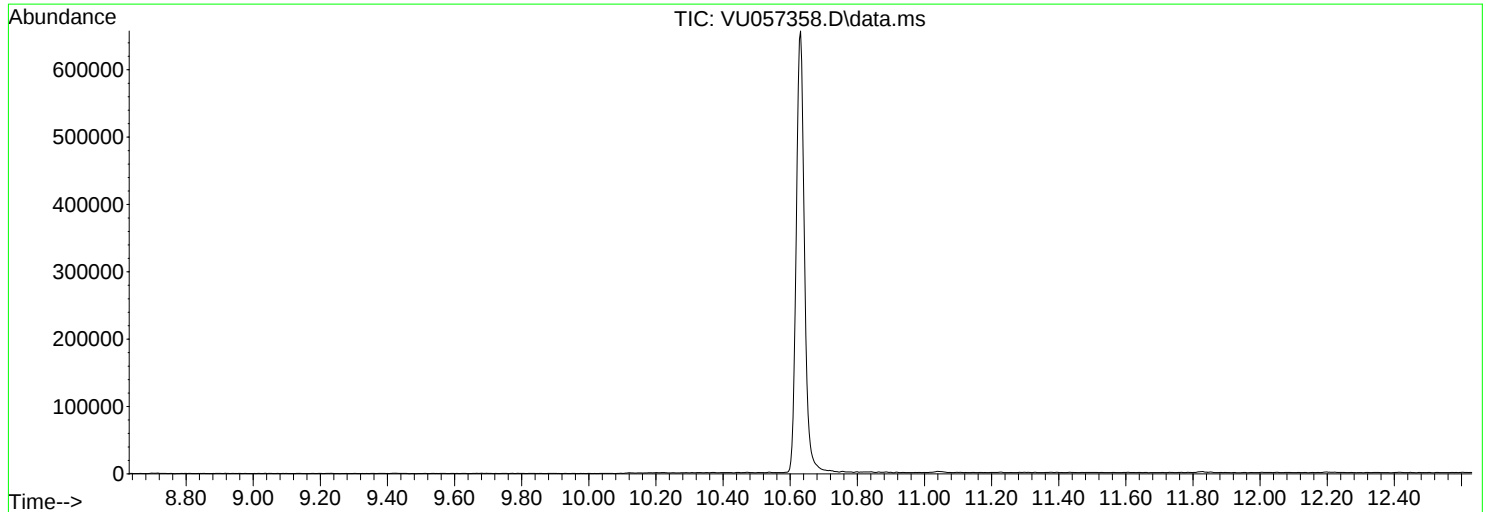

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	23675	PASS
75	95	30	80	50.9	68829	PASS
95	95	100	100	100.0	135243	PASS
96	95	5	9	6.6	8989	PASS
173	174	0.00	2	0.6	537	PASS
174	95	50	120	72.2	97619	PASS
175	174	5	9	7.2	7052	PASS
176	174	95	101	96.7	94421	PASS
177	176	5	9	6.1	5736	PASS

m/z	Abundance
35.90	901.0
37.80	377.0
39.80	325.0
43.90	491.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	1956.0
36.90	5252.0
37.90	5300.0
39.00	2149.0
39.70	273.0
43.80	1056.0
44.90	982.0
46.00	271.0
47.00	1497.0
47.90	743.0
48.90	5118.0
50.00	24464.0
51.00	7260.0
51.90	321.0
52.80	216.0
53.90	182.0
54.90	471.0
55.90	1793.0
56.90	3493.0
58.00	150.0
59.90	1291.0
60.90	6038.0
62.00	6697.0
63.00	6553.0
63.90	1667.0
65.00	1549.0
65.90	200.0
67.00	343.0
68.00	12948.0
69.00	14550.0
70.00	1002.0
71.80	763.0
72.90	5976.0
74.00	22096.0
75.00	70368.0
75.90	6323.0
77.00	998.0
78.90	5577.0
79.90	1445.0
80.90	6084.0
81.90	1103.0
82.90	133.0
85.90	161.0
86.90	5696.0
87.90	5076.0
90.80	479.0
91.90	4064.0
92.90	6375.0
94.00	16568.0
95.00	138240.0
96.00	9093.0
96.90	396.0
103.80	642.0
104.80	178.0
105.80	489.0
106.70	161.0
109.80	126.0
110.90	236.0
111.70	100.0
112.90	131.0
114.80	133.0
115.80	580.0
116.90	1437.0
117.90	635.0
118.90	989.0
123.90	134.0
127.90	527.0
128.80	168.0
129.80	643.0
130.70	191.0
134.70	339.0
136.70	293.0
139.60	142.0
140.90	1814.0
142.90	2448.0
144.90	1242.0
145.70	255.0
147.90	384.0
150.00	104.0
154.80	344.0
157.00	257.0
158.90	152.0
160.90	157.0
170.90	527.0
171.90	1911.0
173.00	1611.0
173.90	95720.0
174.90	6850.0
175.90	94256.0
177.00	5867.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	1924.0
36.90	5231.0
37.90	5255.0
39.00	2286.0
39.70	305.0
43.90	1033.0
45.00	1003.0
46.00	317.0
47.00	1639.0
47.80	758.0
48.90	5588.0
50.00	24512.0
51.00	7384.0
51.90	320.0
52.90	214.0
53.90	224.0
54.90	471.0
55.90	1555.0
56.90	3331.0
57.90	159.0
59.90	1395.0
60.90	6226.0
62.00	6574.0
62.90	6503.0
64.00	1566.0
65.00	1795.0
66.00	174.0
67.00	297.0
68.00	12996.0
69.00	14770.0
70.00	964.0
71.80	846.0
73.00	6184.0
74.00	22912.0
75.00	71264.0
76.00	6390.0
77.00	918.0
78.90	5651.0
79.90	1537.0
80.90	5864.0
81.80	1139.0
82.90	129.0
85.90	127.0
86.90	5849.0
87.90	5290.0
90.80	493.0
91.90	4285.0
92.90	6447.0
94.00	16720.0
95.00	139008.0
96.00	9250.0
96.90	423.0
103.80	580.0
104.80	216.0
105.80	523.0
106.70	201.0
108.00	112.0
109.80	139.0
110.90	206.0
111.80	102.0
113.00	141.0
114.90	137.0
115.80	590.0
116.90	1448.0
117.80	682.0
118.90	1172.0
127.90	460.0
128.70	154.0
129.80	621.0
130.70	182.0
134.70	430.0
136.70	380.0
139.60	148.0
140.10	107.0
140.90	1762.0
141.70	168.0
142.90	2468.0
144.90	1230.0
145.80	229.0
147.00	121.0
147.90	417.0
150.00	133.0
154.80	273.0
156.90	280.0
158.90	164.0
160.90	204.0
170.70	560.0
171.90	2155.0
173.90	100608.0
174.90	7292.0
175.90	97264.0
177.00	5935.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	1918.0
36.90	5074.0
37.90	4788.0
39.00	2236.0
39.70	281.0
40.20	252.0
44.00	917.0
44.90	852.0
46.00	262.0
47.00	1470.0
47.80	701.0
48.90	5223.0
50.00	22048.0
51.00	6945.0
51.90	321.0
52.90	188.0
54.00	234.0
54.90	367.0
55.90	1484.0
56.90	2839.0
57.90	148.0
58.80	105.0
59.90	1250.0
60.90	5957.0
62.00	5854.0
62.90	5890.0
64.00	1302.0
65.00	1768.0
66.00	130.0
67.00	256.0
67.90	11949.0
68.90	13589.0
69.90	803.0
71.90	755.0
72.90	5959.0
74.00	21856.0
75.00	64856.0
76.00	5972.0
77.00	797.0
78.00	431.0
78.90	5259.0
79.90	1526.0
80.90	5108.0
81.80	1108.0
82.90	132.0
86.90	5341.0
87.90	4497.0
90.80	436.0
91.90	4012.0
92.90	5846.0
94.00	15554.0
95.00	128480.0
96.00	8625.0
96.90	420.0
103.80	539.0
104.80	191.0
105.80	554.0
106.70	192.0
108.00	136.0
109.90	146.0
110.90	139.0
113.00	125.0
114.90	134.0
115.80	549.0
116.90	1232.0
117.80	637.0
118.90	1112.0
127.90	363.0
128.70	172.0
129.80	520.0
130.80	164.0
134.70	385.0
136.70	418.0
139.60	133.0
140.90	1515.0
141.70	193.0
142.90	2367.0
144.80	1105.0
146.00	200.0
147.10	126.0
147.90	389.0
150.00	119.0
155.00	277.0
156.90	261.0
158.90	124.0
160.80	187.0
170.80	490.0
171.90	1982.0
173.90	96528.0
174.90	7014.0
175.90	91744.0
177.00	5407.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104