
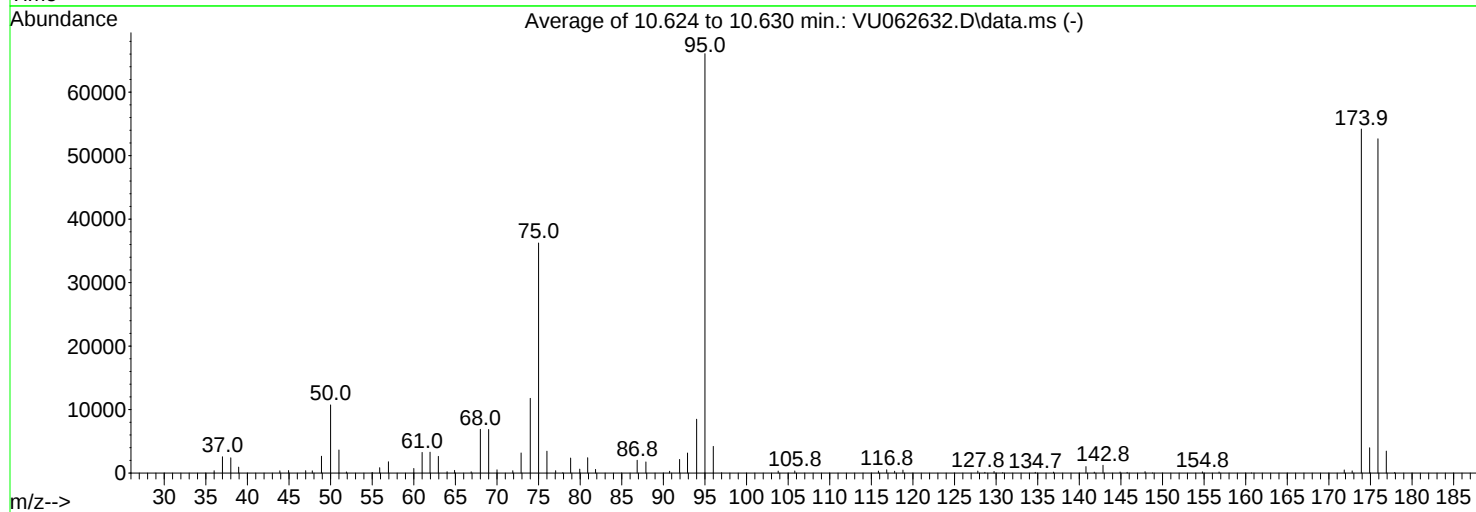


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU123024\
Data File : VU062632.D
Acq On : 30 Dec 2024 08:35
Operator : MD/SY
Sample : BFB055
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB055

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Dec 31 00:16:34 2024

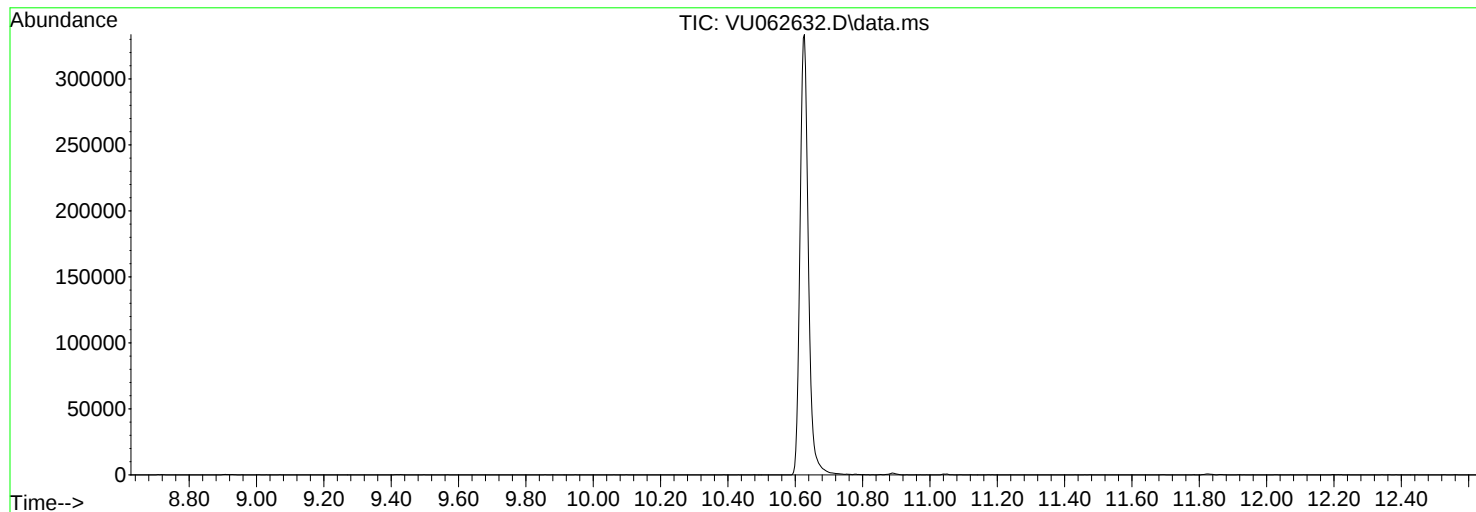

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	10737	PASS
75	95	30	80	54.9	36237	PASS
95	95	100	100	100.0	66056	PASS
96	95	5	9	6.4	4206	PASS
173	174	0.00	2	0.6	349	PASS
174	95	50	120	82.0	54189	PASS
175	174	5	9	7.4	3984	PASS
176	174	95	101	97.2	52653	PASS
177	176	5	9	6.6	3461	PASS

Scan 2890 (10.624 min): VU062632.D\data.ms

BFB055

m/z Abundance

m/z	Abundance
36.00	415.0
37.00	2654.0
38.00	2601.0
38.90	960.0
43.90	378.0
45.00	402.0
47.00	393.0
47.70	390.0
48.90	2761.0
50.00	11197.0
51.00	3769.0
51.90	147.0
55.00	148.0
55.90	906.0
57.00	1893.0
60.00	733.0
61.00	3627.0
61.90	3288.0
63.00	2792.0
64.00	229.0
64.90	461.0
66.90	232.0
68.00	7195.0
69.00	7111.0
70.00	520.0
71.80	380.0
72.90	3353.0
74.00	12332.0
75.00	37200.0
76.00	3557.0
77.00	377.0
77.90	173.0
78.90	2377.0
80.00	656.0
80.90	2453.0
81.80	619.0
86.90	2000.0
87.90	1784.0
90.80	291.0
91.90	2123.0
92.90	3280.0
94.00	8799.0
95.00	67336.0
96.00	4584.0
97.00	116.0
103.80	304.0
105.80	340.0
115.80	309.0
116.80	483.0
117.80	296.0
118.80	430.0
127.80	328.0
128.60	125.0
129.70	248.0
134.70	115.0
136.90	123.0
140.80	1018.0
141.80	173.0
142.80	1136.0
144.90	182.0
145.70	109.0
147.90	241.0
154.80	256.0
156.80	209.0
171.80	524.0
173.90	54472.0
174.90	4048.0
175.90	52824.0
176.90	3477.0
177.90	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
36.00	364.0
37.00	2658.0
38.00	2468.0
38.90	944.0
43.90	354.0
45.00	406.0
47.00	377.0
47.80	373.0
48.90	2737.0
50.00	10932.0
51.00	3769.0
51.90	187.0
55.00	117.0
55.90	872.0
56.90	1816.0
60.00	765.0
61.00	3342.0
62.00	3379.0
63.00	2719.0
64.10	212.0
64.90	443.0
66.90	220.0
68.00	7194.0
69.00	7059.0
70.00	555.0
71.90	381.0
72.90	3283.0
74.00	12001.0
75.00	37240.0
76.00	3563.0
77.00	422.0
78.80	2408.0
79.90	636.0
80.90	2473.0
81.80	601.0
86.90	2078.0
87.90	1796.0
90.80	292.0
91.90	2194.0
92.90	3251.0
94.00	8682.0
95.00	67968.0
96.00	4396.0
103.80	332.0
105.80	338.0
115.80	323.0
116.90	552.0
117.80	289.0
118.80	497.0
127.80	340.0
128.60	126.0
129.70	247.0
130.80	108.0
134.70	126.0
136.90	163.0
140.80	1069.0
141.80	163.0
142.90	1292.0
144.90	184.0
145.70	130.0
147.90	238.0
154.80	201.0
156.80	191.0
171.80	502.0
172.80	546.0
173.90	55792.0
174.90	4060.0
175.90	54104.0
176.90	3581.0
177.90	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
36.00	337.0
37.00	2414.0
38.00	2152.0
39.00	916.0
43.90	342.0
44.90	394.0
47.00	370.0
47.90	311.0
48.90	2473.0
50.00	10083.0
51.00	3392.0
51.90	213.0
55.90	767.0
56.90	1657.0
60.00	682.0
61.00	2789.0
62.00	3198.0
62.90	2384.0
63.90	219.0
64.90	364.0
66.90	180.0
68.00	6292.0
69.00	6435.0
70.00	471.0
72.00	354.0
72.90	2883.0
74.00	10995.0
75.00	34272.0
76.00	3232.0
77.10	346.0
78.90	2315.0
79.90	567.0
80.90	2327.0
81.90	518.0
86.80	1989.0
87.90	1675.0
90.70	290.0
92.00	2121.0
92.90	2971.0
94.00	7959.0
95.00	62864.0
96.00	3638.0
103.80	329.0
105.80	320.0
115.90	315.0
116.90	532.0
117.80	292.0
118.80	518.0
127.80	288.0
128.70	125.0
129.80	281.0
130.80	137.0
134.70	131.0
136.90	181.0
140.80	981.0
141.80	125.0
142.90	1271.0
144.90	171.0
145.80	129.0
147.90	198.0
148.80	102.0
154.80	137.0
156.80	127.0
160.70	101.0
171.90	443.0
172.80	500.0
173.90	52304.0
174.90	3844.0
175.90	51032.0
176.90	3324.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055