
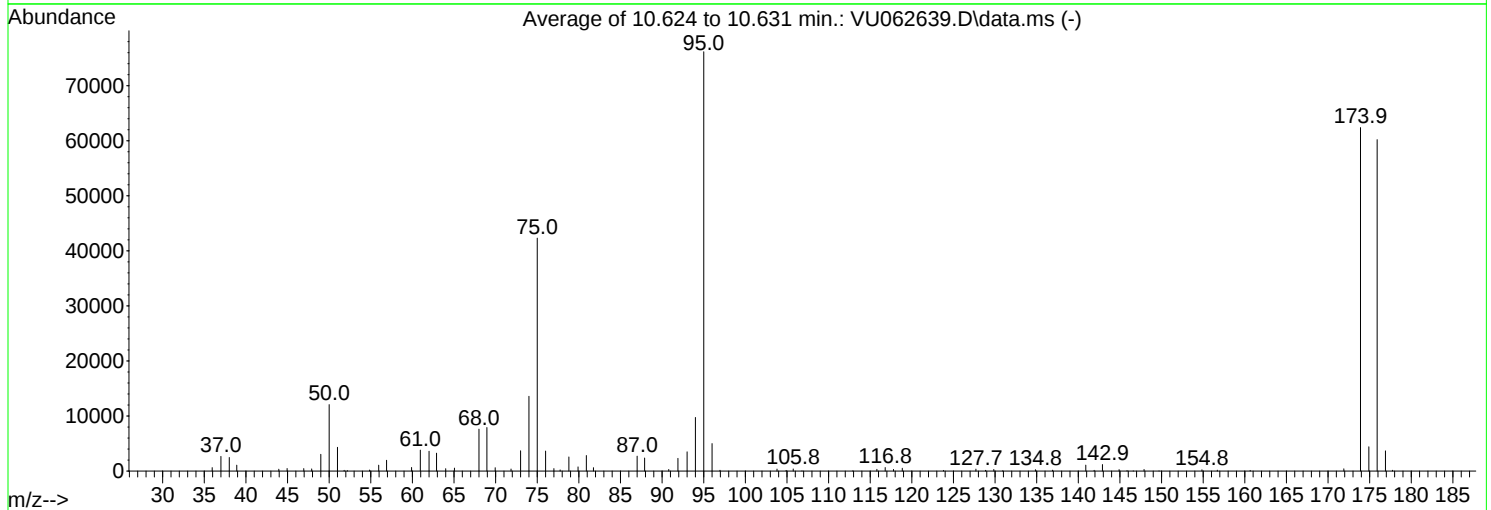


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU123124\
Data File : VU062639.D
Acq On : 31 Dec 2024 08:59
Operator : MD/SY
Sample : BFB056
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB056

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jan 01 00:16:18 2025

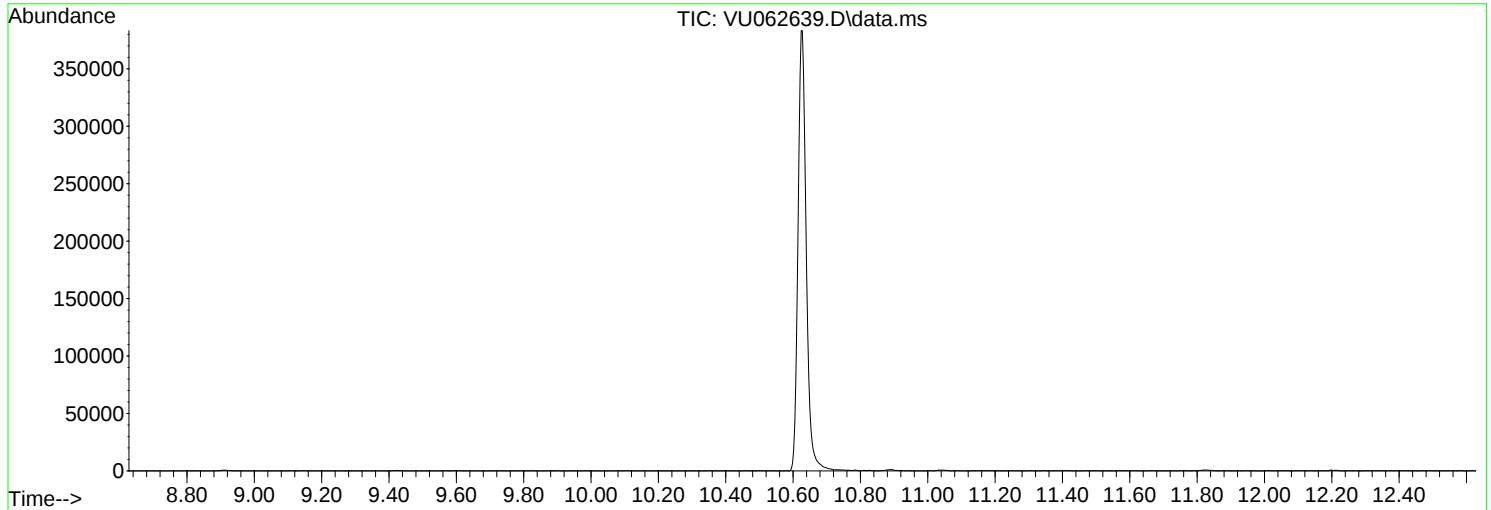

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	12080	PASS
75	95	30	80	55.5	42312	PASS
95	95	100	100	100.0	76173	PASS
96	95	5	9	6.6	4995	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.9	62395	PASS
175	174	5	9	7.1	4411	PASS
176	174	95	101	96.5	60205	PASS
177	176	5	9	6.1	3673	PASS

m/z	Abundance
44.00	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
35.90	524.0
37.00	2868.0
38.00	2584.0
38.90	1107.0
44.00	470.0
45.00	549.0
47.00	457.0
47.90	383.0
49.00	3220.0
50.00	12400.0
51.00	4463.0
51.90	147.0
55.00	251.0
55.90	1185.0
56.90	2055.0
59.90	730.0
60.90	3787.0
62.00	3700.0
62.90	3424.0
64.00	421.0
65.00	547.0
68.00	7836.0
69.00	8257.0
70.00	582.0
72.00	415.0
73.00	3813.0
74.00	14075.0
75.00	44624.0
76.00	3829.0
77.00	495.0
77.70	208.0
78.80	2670.0
79.90	814.0
80.90	3125.0
81.80	661.0
87.00	3090.0
87.90	2491.0
90.80	285.0
91.90	2356.0
93.00	3755.0
94.00	9927.0
95.00	78592.0
96.00	5303.0
96.90	168.0
103.80	364.0
104.90	104.0
105.80	372.0
115.80	340.0
116.80	671.0
117.80	260.0
118.80	507.0
123.80	115.0
127.70	321.0
128.90	177.0
129.80	315.0
130.90	145.0
134.80	234.0
136.90	199.0
140.90	1142.0
141.90	107.0
142.90	1132.0
144.90	258.0
147.90	325.0
154.90	237.0
156.70	128.0
160.70	111.0
171.90	429.0
173.90	62816.0
174.90	4596.0
175.90	61352.0
176.90	3728.0
177.80	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
36.00	648.0
37.00	2719.0
38.00	2559.0
38.90	1111.0
43.90	478.0
44.90	478.0
47.00	448.0
47.90	401.0
49.00	3165.0
50.00	12327.0
51.00	4512.0
51.80	147.0
52.20	128.0
54.80	187.0
56.00	1101.0
56.90	1990.0
59.90	643.0
60.90	3867.0
62.00	3640.0
62.90	3359.0
64.00	442.0
65.00	547.0
68.00	7834.0
69.00	8123.0
70.00	649.0
71.80	384.0
73.00	3805.0
74.00	13922.0
75.00	43488.0
76.00	3693.0
77.00	482.0
77.70	224.0
78.80	2643.0
79.90	779.0
80.90	2908.0
81.80	662.0
87.00	2821.0
87.90	2438.0
90.80	316.0
91.90	2422.0
93.00	3577.0
94.00	10059.0
95.00	78656.0
96.00	5078.0
96.90	150.0
103.80	371.0
104.90	134.0
105.80	395.0
112.90	104.0
115.80	335.0
116.80	674.0
117.80	310.0
118.90	525.0
123.80	149.0
127.70	381.0
128.80	149.0
129.80	298.0
134.90	270.0
136.90	174.0
140.90	1107.0
141.90	147.0
142.90	1214.0
144.90	296.0
145.90	110.0
146.60	108.0
147.90	323.0
154.90	257.0
156.70	163.0
160.70	126.0
171.90	409.0
173.90	64120.0
174.90	4524.0
175.90	62016.0
176.90	3708.0
177.70	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
36.00	703.0
37.00	2404.0
38.00	2273.0
38.90	1015.0
44.00	429.0
45.00	383.0
46.80	469.0
47.90	398.0
49.00	2749.0
50.00	11514.0
51.00	3985.0
51.70	121.0
52.20	105.0
54.80	158.0
56.00	942.0
56.90	1849.0
59.90	585.0
61.00	3769.0
62.00	3464.0
62.90	2979.0
64.00	443.0
65.10	534.0
68.00	7212.0
68.90	7350.0
69.90	604.0
71.80	339.0
73.00	3448.0
74.00	12763.0
75.00	38824.0
76.00	3373.0
77.00	395.0
77.80	202.0
78.80	2382.0
79.90	689.0
80.90	2445.0
81.70	540.0
87.00	2244.0
87.90	2192.0
90.80	308.0
91.90	2156.0
93.00	3157.0
94.00	9239.0
95.00	71272.0
96.00	4603.0
97.00	138.0
103.80	357.0
104.90	127.0
105.70	385.0
106.80	117.0
115.80	286.0
116.80	593.0
117.80	329.0
118.90	504.0
123.80	118.0
127.70	374.0
128.80	105.0
129.90	289.0
134.90	253.0
136.90	135.0
140.90	990.0
141.90	181.0
142.90	1205.0
144.90	267.0
145.80	144.0
147.90	257.0
149.70	101.0
154.80	222.0
156.70	201.0
160.60	127.0
171.90	407.0
173.90	60248.0
174.90	4114.0
175.90	57248.0
176.90	3584.0
177.70	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056