


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010419\
 Data File : VV009153.D
 Acq On : 04 Jan 2019 09:56
 Operator : SY/MD
 Sample : BFB68
 Misc : 5.00 G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB68

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM010419S.M
 Title : VOC Analysis
 Last Update : Sat Jan 05 05:00:49 2019

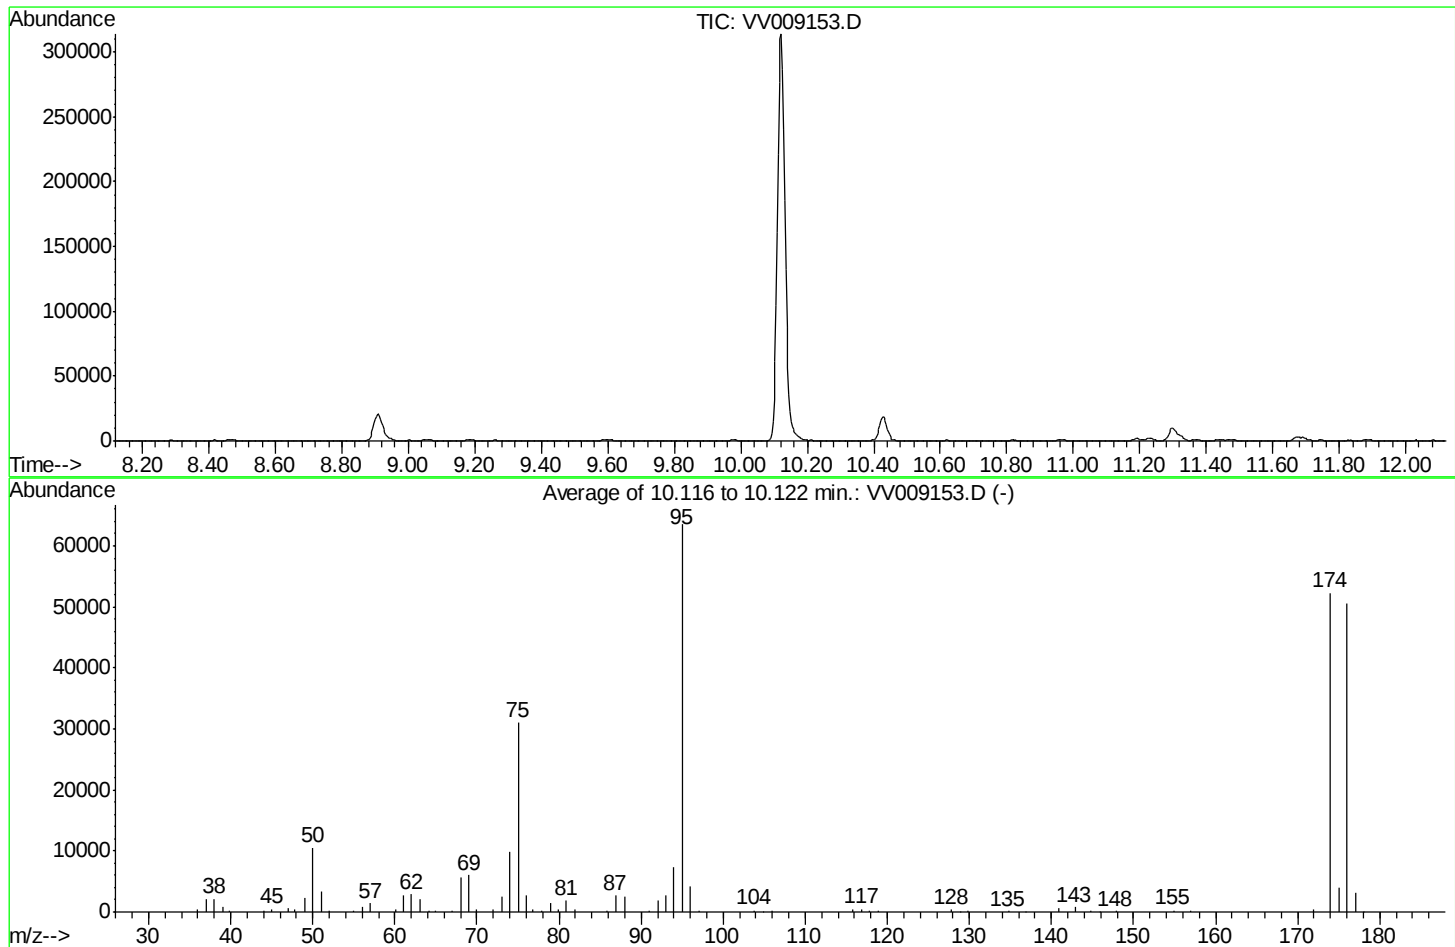

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	10585	PASS
75	95	30	80	48.8	30994	PASS
95	95	100	100	100.0	63528	PASS
96	95	5	9	6.7	4241	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.3	52258	PASS
175	174	5	9	7.8	4058	PASS
176	174	95	101	96.6	50472	PASS
177	176	5	9	6.2	3125	PASS

m/z	Abundance
35.90	395.0
37.00	1998.0
38.00	2031.0
39.00	833.0
39.90	106.0
44.10	464.0
45.00	389.0
47.00	601.0
47.90	370.0
49.00	2084.0
50.00	9838.0
51.00	3066.0
51.90	200.0
55.00	172.0
56.00	856.0
57.00	1277.0
60.10	535.0
61.00	2544.0
62.00	2691.0
63.00	2064.0
64.10	218.0
64.90	327.0
67.00	200.0
68.00	5556.0
69.00	5686.0
70.00	355.0
71.90	338.0
73.00	2499.0
74.00	9000.0
75.00	28952.0
76.00	2380.0
76.80	361.0
77.80	273.0
78.90	1468.0
79.90	443.0
80.90	1713.0
81.90	345.0
85.80	150.0
86.90	2400.0
88.00	2360.0
91.00	295.0
92.00	1657.0
93.00	2468.0
94.00	6860.0
95.00	59352.0
96.00	3873.0
97.10	116.0
103.90	232.0
105.90	219.0
115.70	285.0
117.00	428.0
117.90	257.0
118.80	314.0
127.80	309.0
129.80	234.0
134.90	103.0
141.00	517.0
142.90	732.0
144.90	131.0
145.90	102.0
147.90	160.0
154.90	237.0
157.00	130.0
172.10	487.0
174.00	47096.0
175.00	3766.0
176.00	45112.0
177.00	3016.0
178.00	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	440.0
37.00	2180.0
38.00	2202.0
39.00	919.0
39.90	110.0
44.10	465.0
45.00	442.0
47.10	633.0
47.80	372.0
49.00	2357.0
50.00	10965.0
51.00	3419.0
51.90	231.0
55.00	183.0
56.00	898.0
57.00	1451.0
60.10	519.0
61.00	2719.0
62.00	3011.0
63.00	2285.0
64.10	260.0
65.00	312.0
67.00	243.0
68.00	5891.0
69.00	6261.0
69.90	393.0
71.90	393.0
73.00	2734.0
74.00	10111.0
75.00	31848.0
76.00	2800.0
76.80	416.0
77.80	274.0
78.90	1576.0
79.90	503.0
80.90	1967.0
81.90	420.0
85.90	155.0
86.90	2803.0
88.00	2607.0
91.00	352.0
92.00	2017.0
93.00	2831.0
94.00	7603.0
95.00	65880.0
96.00	4379.0
97.10	167.0
103.80	250.0
105.90	219.0
115.80	344.0
116.90	493.0
117.80	277.0
118.90	314.0
127.80	362.0
128.90	118.0
129.80	269.0
134.80	113.0
140.90	629.0
142.90	870.0
144.80	168.0
145.90	114.0
147.90	180.0
154.90	276.0
156.90	134.0
172.00	485.0
174.00	54016.0
175.00	4231.0
176.00	52112.0
177.00	3210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
36.00	437.0
37.00	2189.0
38.00	2197.0
39.00	946.0
39.80	127.0
44.00	469.0
45.00	468.0
47.10	548.0
47.80	352.0
49.00	2402.0
50.00	10952.0
51.00	3433.0
52.00	190.0
54.90	164.0
56.00	883.0
57.00	1475.0
60.00	468.0
61.00	2715.0
62.00	2982.0
63.00	2215.0
64.10	302.0
64.90	266.0
67.00	225.0
68.00	5684.0
69.00	6252.0
70.00	370.0
71.90	409.0
73.00	2657.0
74.00	10493.0
75.00	32184.0
76.00	2878.0
76.80	373.0
77.90	200.0
78.90	1563.0
79.90	543.0
80.90	1945.0
81.90	446.0
85.90	126.0
86.90	2747.0
88.00	2532.0
90.90	313.0
92.00	2076.0
93.00	2805.0
94.00	7743.0
95.00	65352.0
96.00	4472.0
97.00	156.0
103.80	232.0
104.80	107.0
105.90	221.0
115.80	365.0
116.90	469.0
117.80	263.0
118.90	336.0
127.80	311.0
128.80	144.0
129.80	275.0
134.70	122.0
136.80	139.0
140.90	751.0
142.90	899.0
144.80	156.0
145.90	102.0
147.90	170.0
154.90	268.0
156.80	101.0
171.90	470.0
174.00	55664.0
175.00	4179.0
176.00	54192.0
177.00	3151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
43.90	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68