
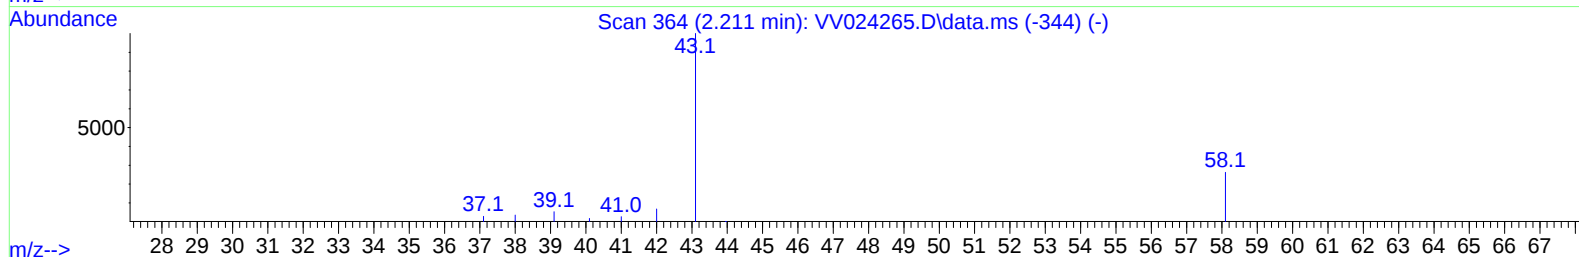
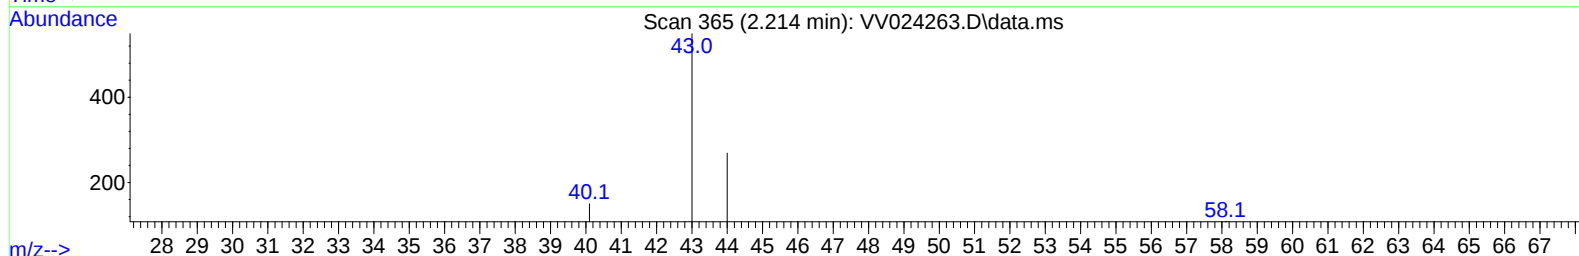


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
 Data File : VV024263.D
 Acq On : 04 Jan 2022 10:37
 Operator : SY/MD
 Sample : VSTD0.571
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jan 04 12:47:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 04 12:47:00 2022
 Response via : Initial Calibration

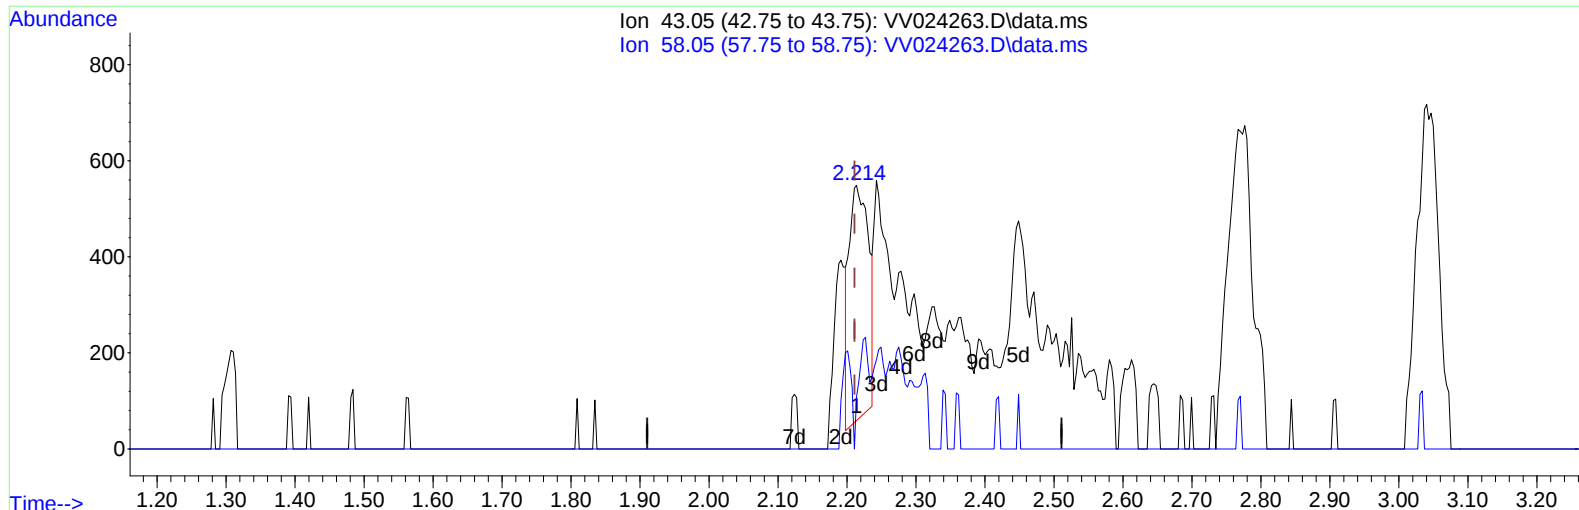

TIC: VV024263.D\data.ms

(13) Acetone (T)

2.214min (+ 0.003) 1.23 ug/L

response 958

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	24.32
0.00	0.00	0.00
0.00	0.00	0.00