
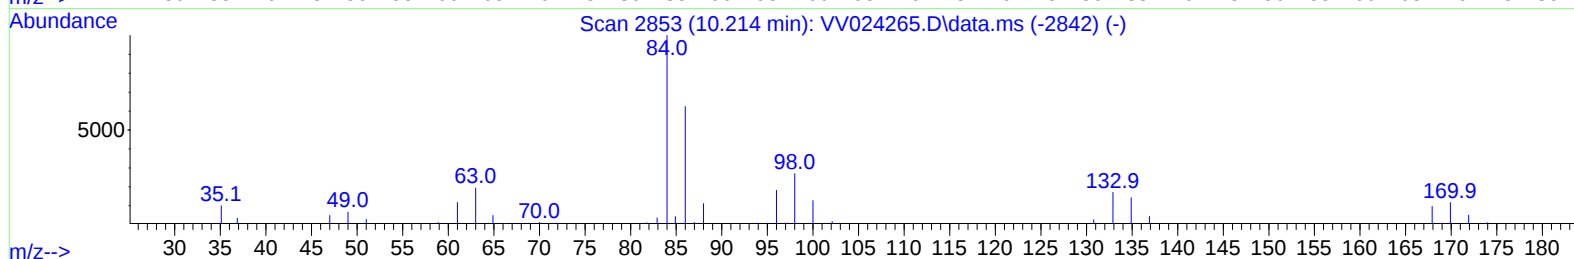
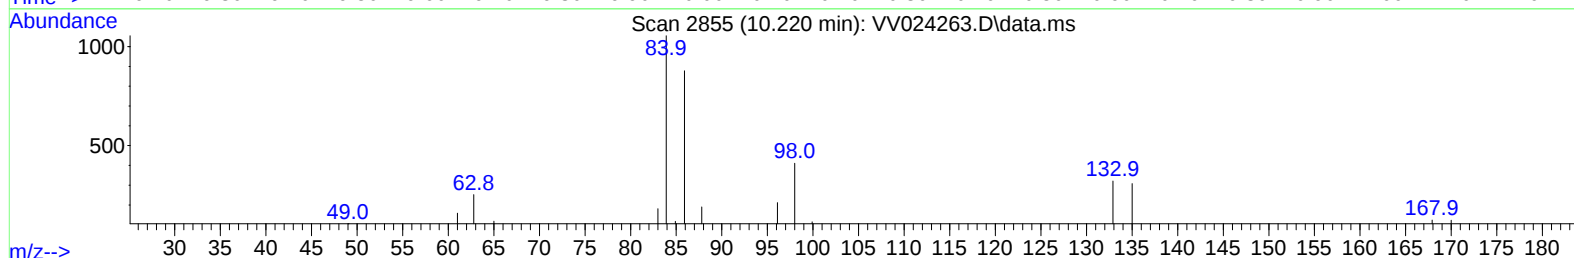


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
Data File : VV024263.D
Acq On : 04 Jan 2022 10:37
Operator : SY/MD
Sample : VSTD0.571
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jan 04 12:47:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 04 12:47:00 2022
Response via : Initial Calibration

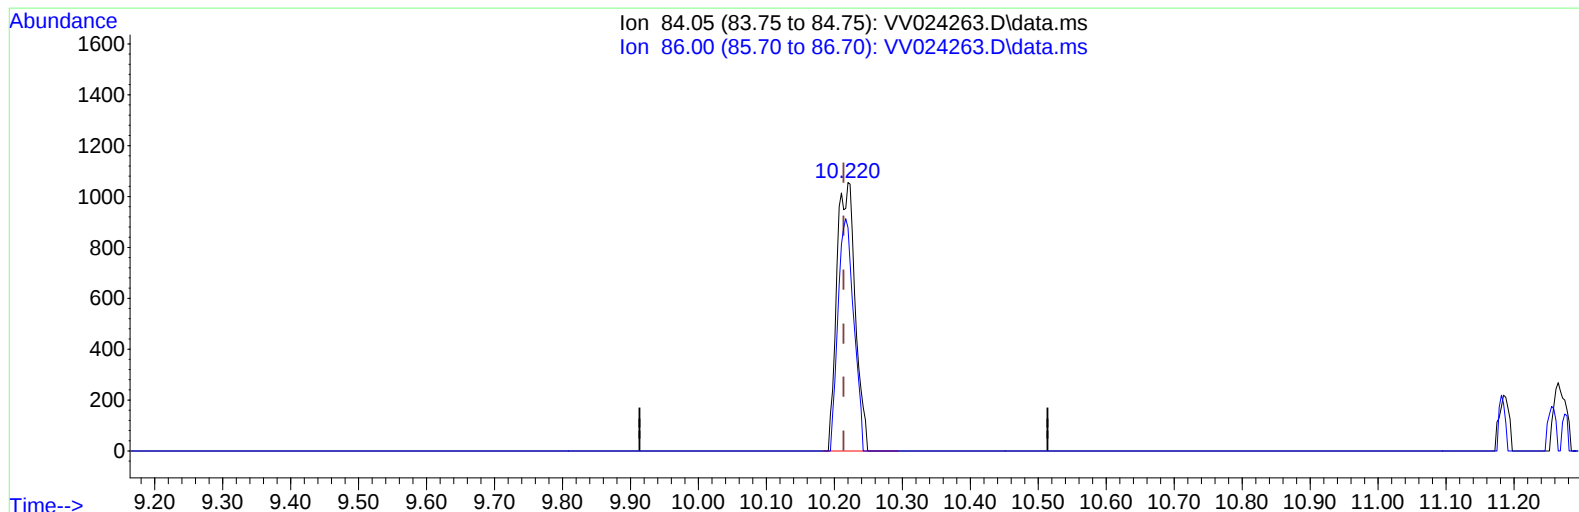

TIC: VV024263.D\data.ms

(56) 1,1,2,2-Tetrachloroethane-d2 (S)

10.220min (+ 0.006) 0.45 ug/L m

response 1987

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	64.70	74.08
0.00	0.00	0.00
0.00	0.00	0.00