
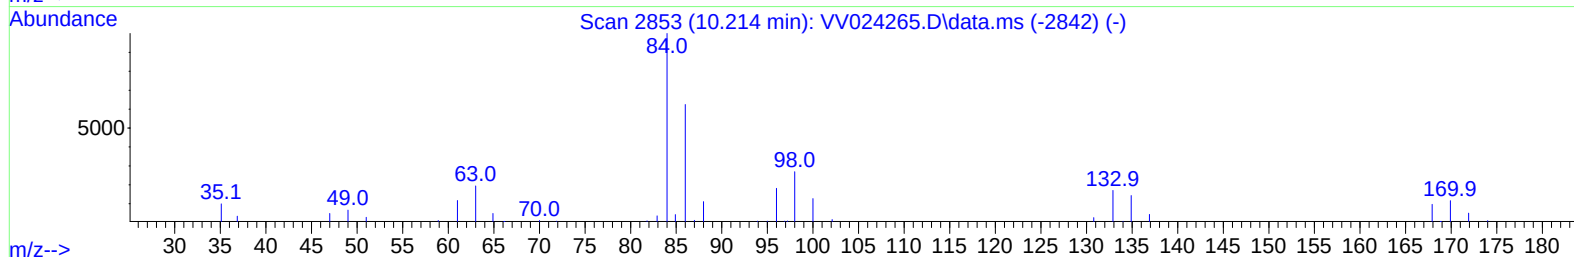
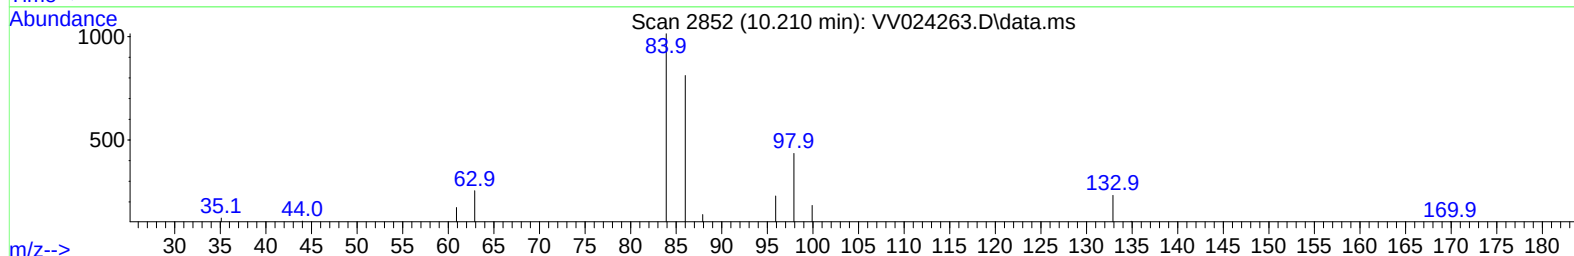


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
 Data File : VV024263.D
 Acq On : 04 Jan 2022 10:37
 Operator : SY/MD
 Sample : VSTD0.571
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jan 04 12:47:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 04 12:47:00 2022
 Response via : Initial Calibration

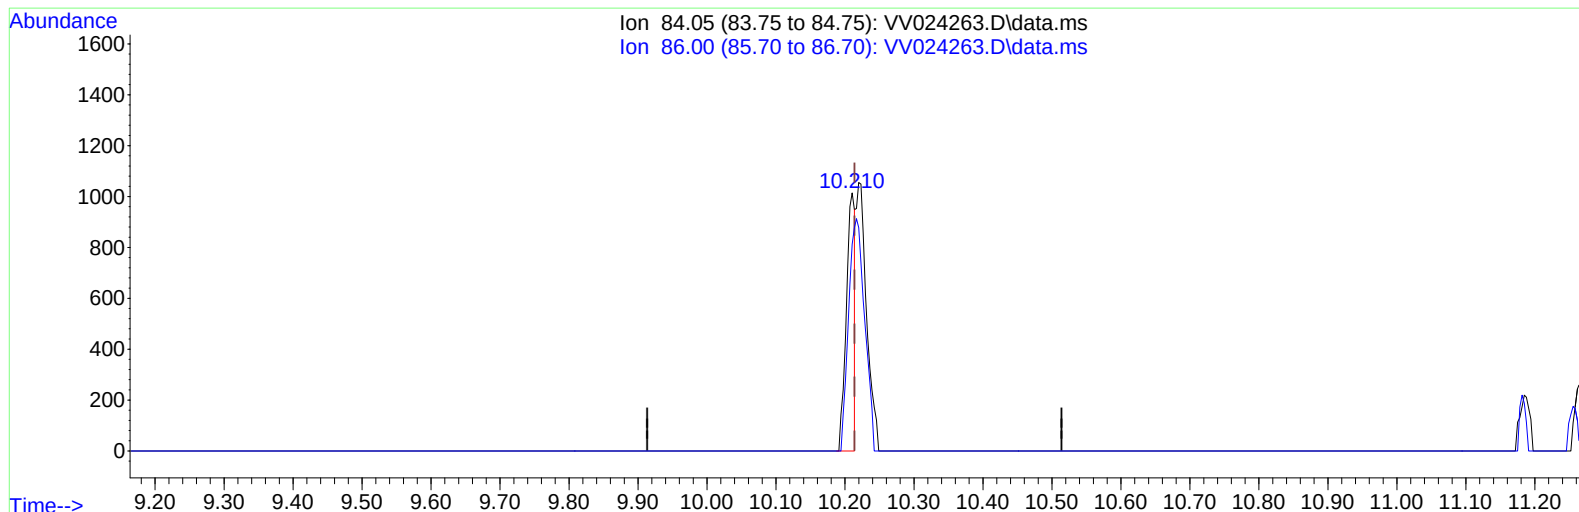

TIC: VV024263.D\data.ms

(56) 1,1,2,2-Tetrachloroethane-d2 (S)**10.210min (-0.003) 0.19 ug/L****response 862**

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	64.70	170.77#
0.00	0.00	0.00
0.00	0.00	0.00