
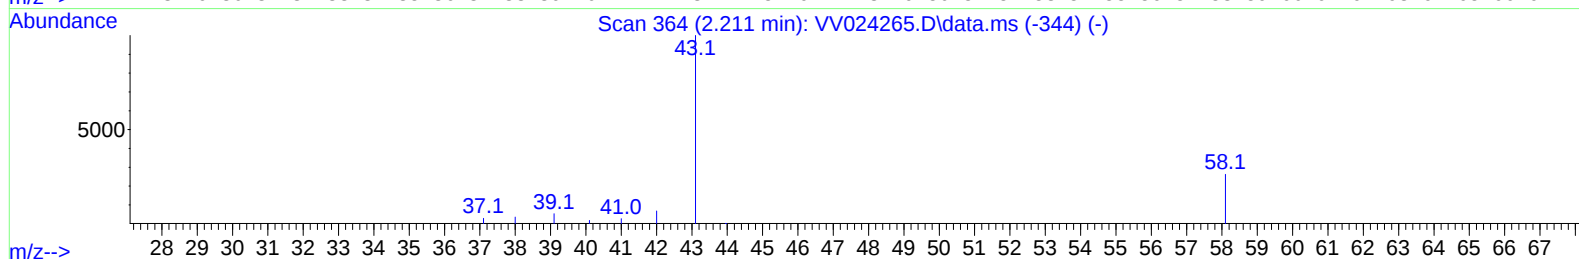
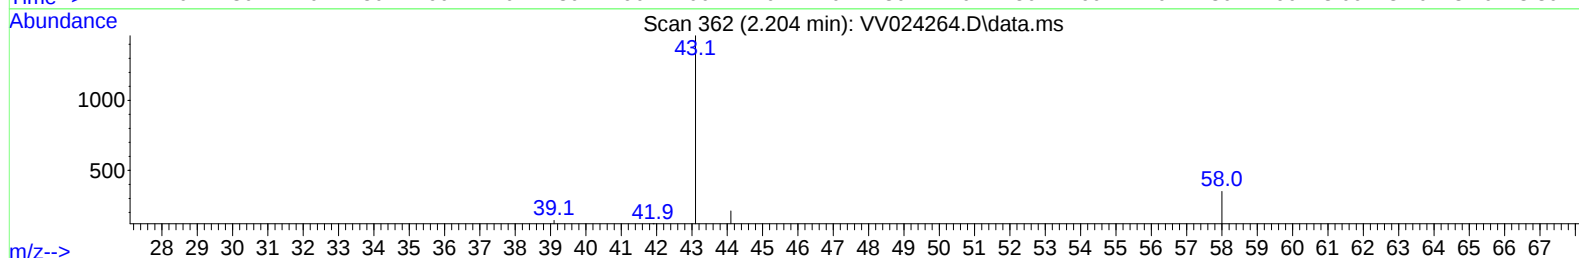


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
 Data File : VV024264.D
 Acq On : 04 Jan 2022 11:31
 Operator : SY/MD
 Sample : VSTD00172
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jan 04 12:47:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 04 12:47:00 2022
 Response via : Initial Calibration

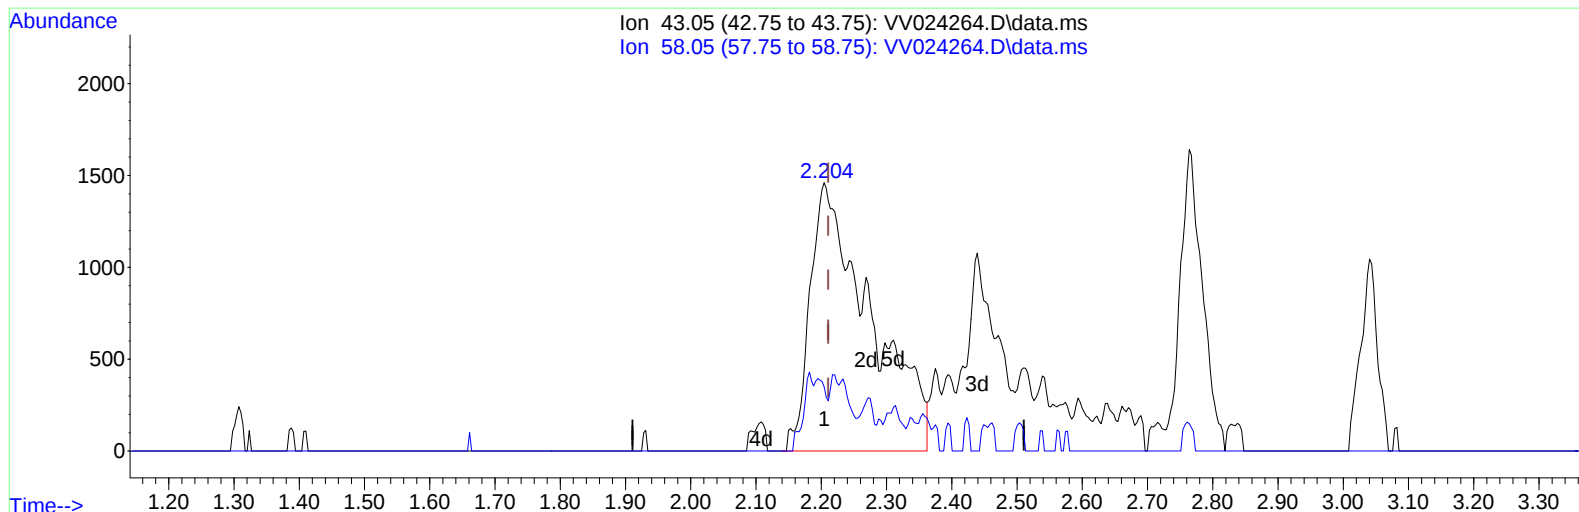

TIC: VV024264.D\data.ms

(13) Acetone (T)

2.204min (-0.006) 11.15 ug/L m

response 9286

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	1.11
0.00	0.00	0.00
0.00	0.00	0.00