
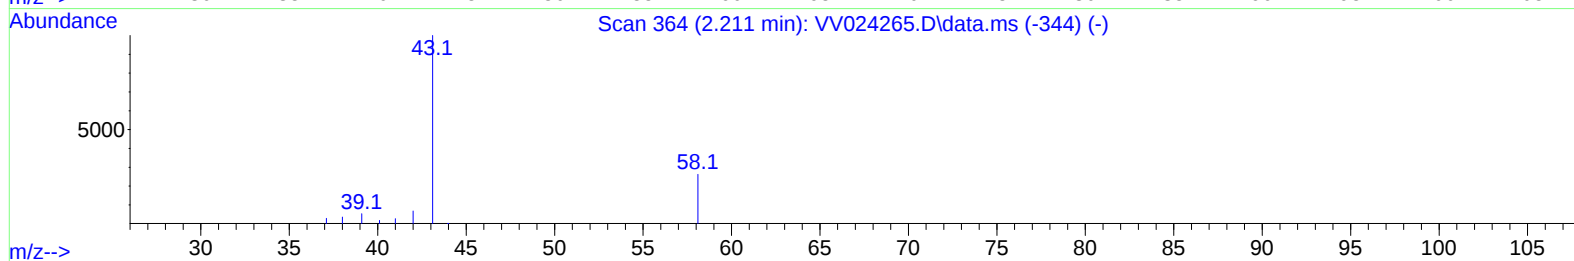
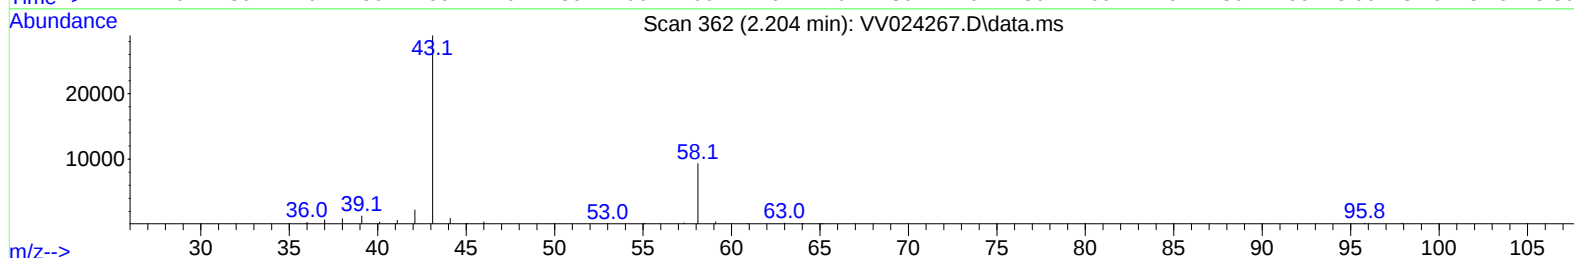


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
 Data File : VV024267.D
 Acq On : 04 Jan 2022 12:42
 Operator : SY/MD
 Sample : VSTD02075
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jan 04 18:30:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 04 13:10:27 2022
 Response via : Initial Calibration

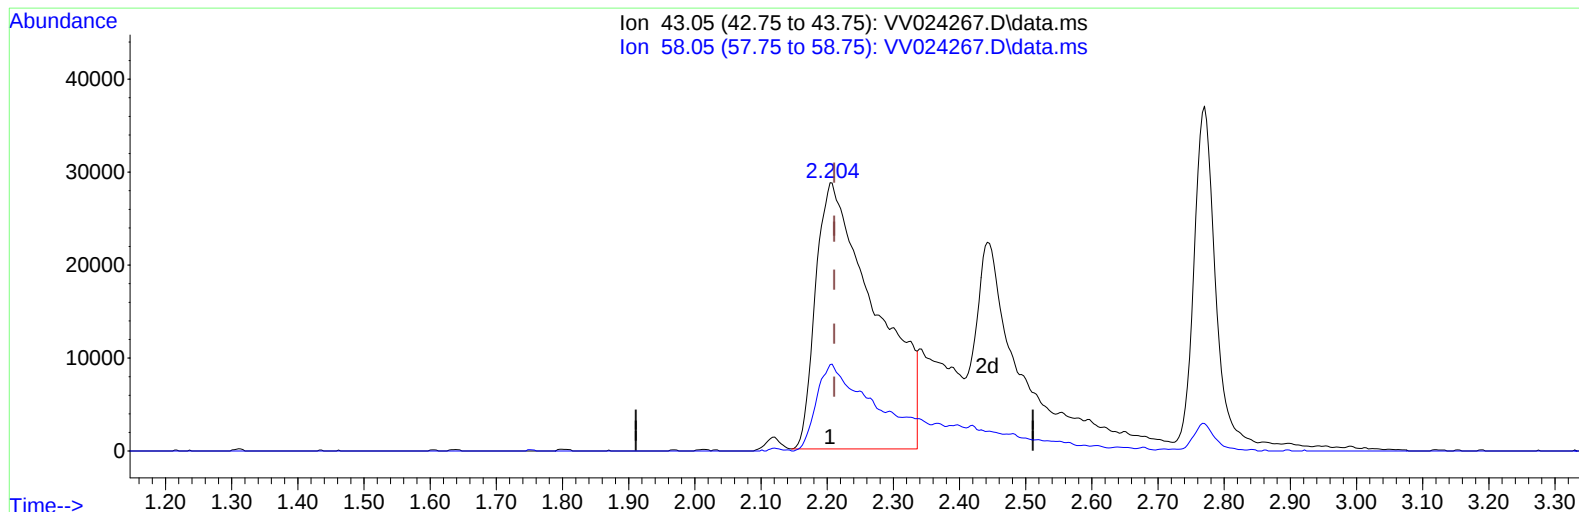

TIC: VV024267.D\data.ms

(13) Acetone (T)

2.204min (-0.007) 173.82 ug/L

response 180043

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	25.61
0.00	0.00	0.00
0.00	0.00	0.00