
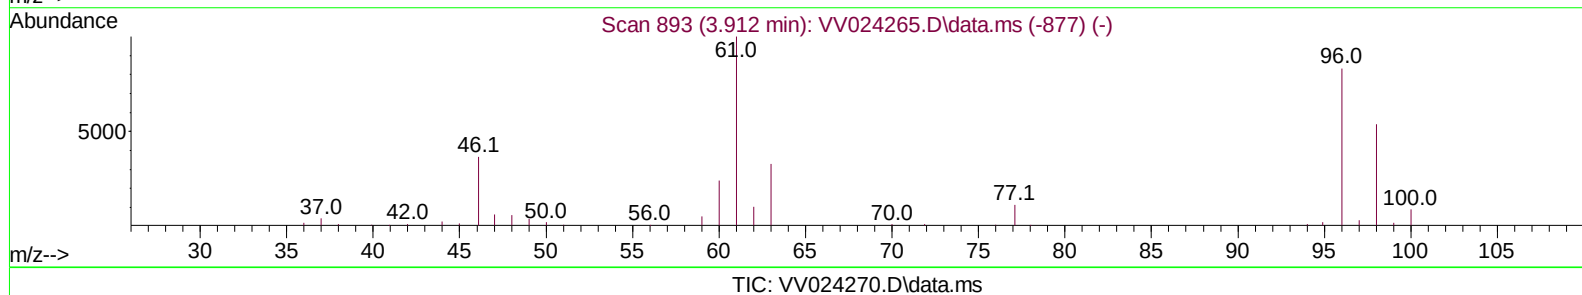
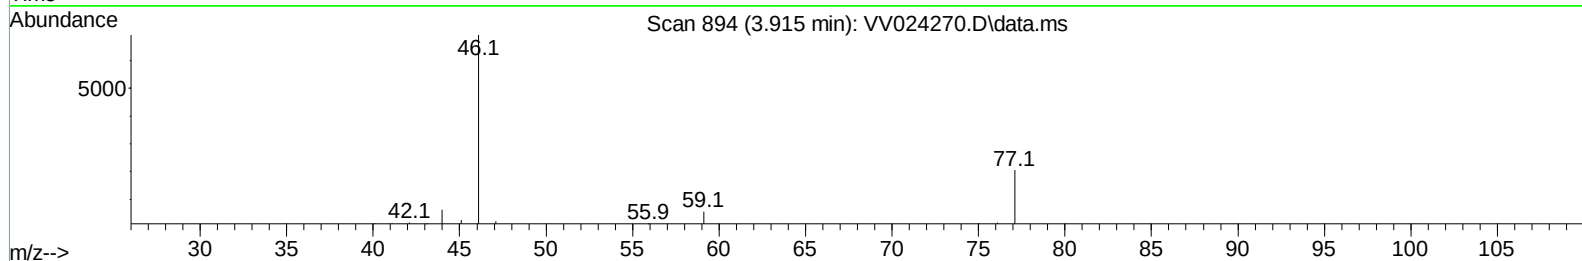


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
Data File : VV024270.D
Acq On : 04 Jan 2022 16:41
Operator : SY/MD
Sample : VV0104WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jan 05 00:40:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 04 18:34:35 2022
Response via : Initial Calibration

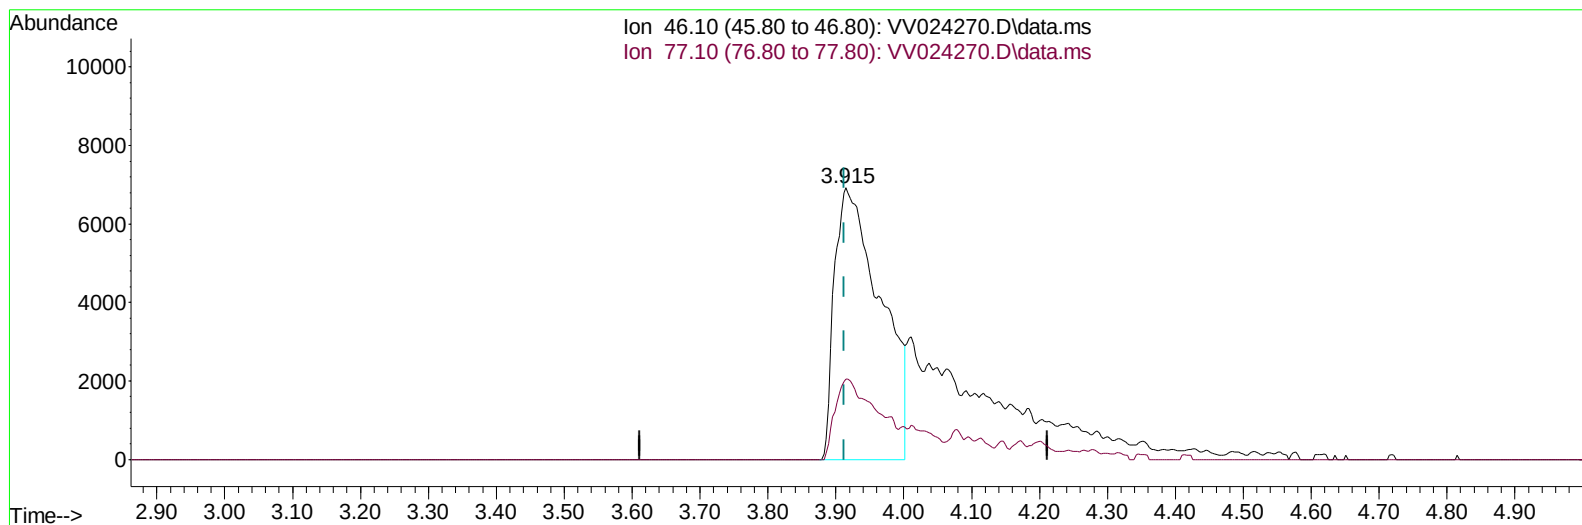

(20) 2-Butanone-d5 (S)




3.915min (+ 0.003) 31.79 ug/L

response 32711

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	26.78#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
 Data File : VV024270.D
 Acq On : 04 Jan 2022 16:41
 Operator : SY/MD
 Sample : VV0104WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jan 05 00:40:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 04 18:34:35 2022
 Response via : Initial Calibration

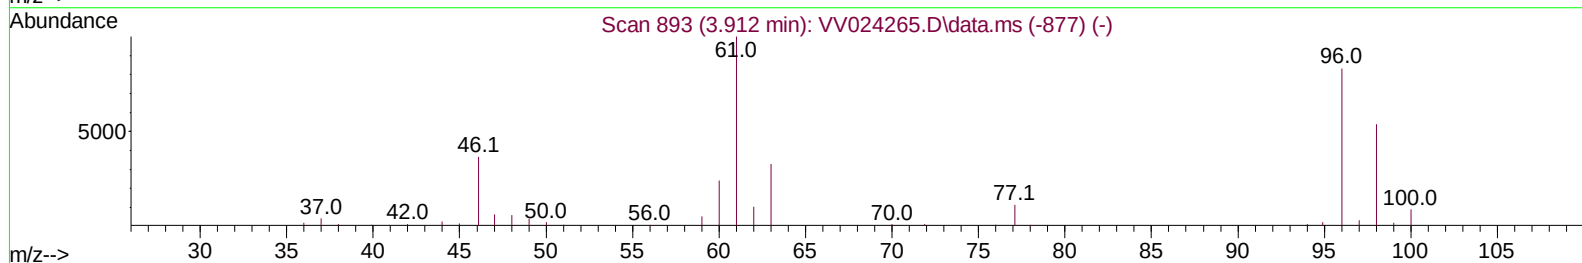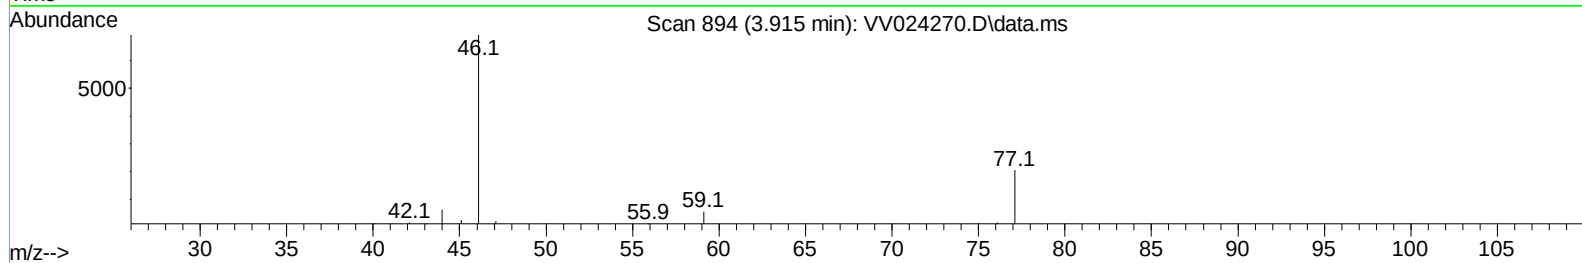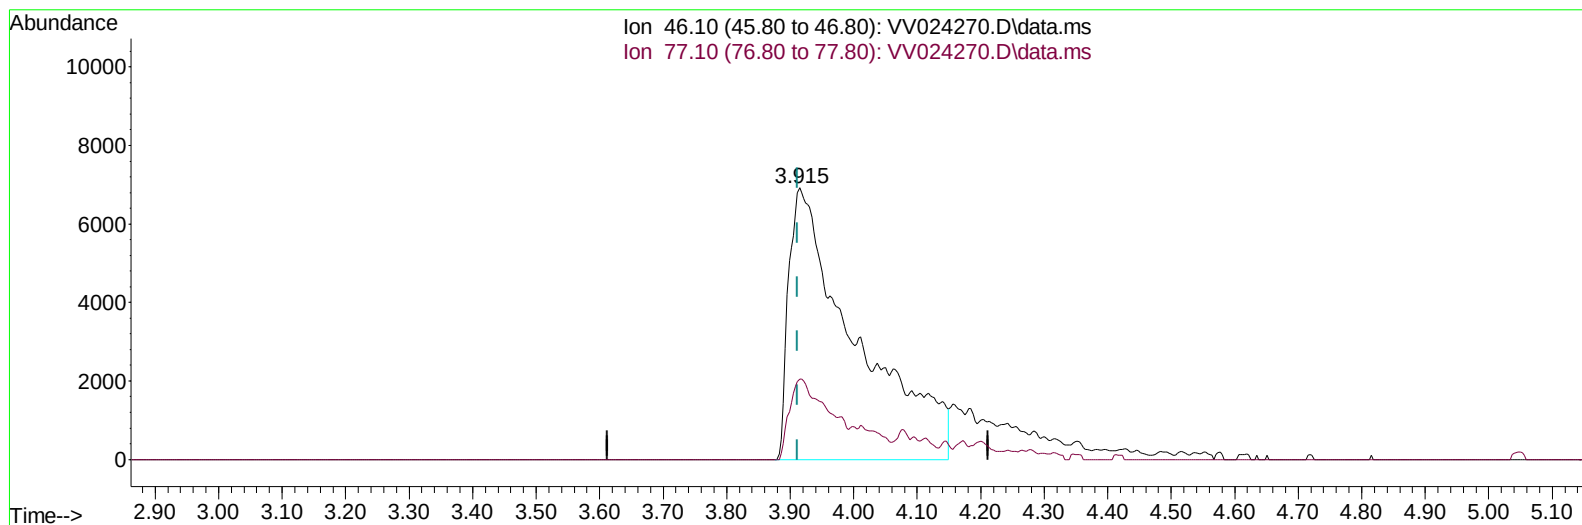

TIC: VV024270.D\data.ms

(20) 2-Butanone-d5 (S)**3.915min (+ 0.003) 49.01 ug/L m****response 50421**

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	17.37#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
 Data File : VV024270.D
 Acq On : 04 Jan 2022 16:41
 Operator : SY/MD
 Sample : VV0104WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jan 05 00:40:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 04 18:34:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	97453	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	99103	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50597	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	37631	4.754	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	95.000%		
7) Chloroethane-d5	1.568	69	29728	4.778	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	95.600%		
11) 1,1-Dichloroethene-d2	2.108	63	55568	3.580	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	71.600%		
20) 2-Butanone-d5	3.915	46	50421m	49.006	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	98.020%		
24) Chloroform-d	4.342	84	71013	4.789	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	95.800%		
26) 1,2-Dichloroethane-d4	5.030	65	35219	5.021	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	100.400%		
32) Benzene-d6	5.046	84	134263	4.836	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	96.800%		
36) 1,2-Dichloropropane-d6	6.066	67	34630	4.800	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	96.000%		
41) Toluene-d8	7.313	98	121974	4.424	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	88.400%		
43) trans-1,3-Dichloroprop...	7.622	79	15300	4.629	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	92.600%		
46) 2-Hexanone-d5	8.088	63	45973	44.512	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	89.020%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	22604	4.305	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	86.000%		
66) 1,2-Dichlorobenzene-d4	11.622	152	48443	5.512	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	110.200%		
Target Compounds						
16) Methylene chloride	2.506	84	6588	0.559	ug/L	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
Data File : VV024270.D
Acq On : 04 Jan 2022 16:41
Operator : SY/MD
Sample : VV0104WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jan 05 00:40:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 04 18:34:35 2022
Response via : Initial Calibration

