

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
 Data File : VV024269.D
 Acq On : 04 Jan 2022 16:06
 Operator : SY/MD
 Sample : VV0104WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK287

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	84662	83893	17.30%	2.134%
2	1.568	156	164	178	rBV	67482	76132	15.70%	1.937%
3	2.108	321	332	355	rVB	148471	211609	43.64%	5.383%
4	2.507	446	456	469	rVB2	13176	23165	4.78%	0.589%
5	3.040	613	622	631	rBV6	3696	6914	1.43%	0.176%
6	3.912	882	893	913	rBV2	16600	65896	13.59%	1.676%
7	4.342	1012	1027	1054	rVB	90407	222797	45.95%	5.668%
8	5.043	1229	1245	1271	rBV2	194242	484877	100.00%	12.335%
9	5.612	1410	1422	1452	rBV	146404	298123	61.48%	7.584%
10	5.908	1503	1514	1526	rBB7	3868	7573	1.56%	0.193%
11	6.066	1549	1563	1584	rBV2	106204	220009	45.37%	5.597%
12	6.982	1838	1848	1871	rBV	55699	106853	22.04%	2.718%
13	7.313	1938	1951	1970	rBV	249790	437323	90.19%	11.125%
14	7.391	1971	1975	1989	rVB4	3355	6263	1.29%	0.159%
15	7.619	2037	2046	2063	rBV2	34566	60408	12.46%	1.537%
16	8.088	2182	2192	2234	rBV	143425	358647	73.97%	9.124%
17	8.850	2417	2429	2451	rBV	228168	371906	76.70%	9.461%
18	10.214	2839	2853	2870	rBV	69499	112406	23.18%	2.859%
19	11.246	3164	3174	3202	rBV	249262	389378	80.30%	9.905%
20	11.622	3279	3291	3314	rBV	239348	386842	79.78%	9.841%




Sum of corrected areas: 3931014

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
Data File : VV024269.D
Acq On : 04 Jan 2022 16:06
Operator : SY/MD
Sample : VV0104WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK287

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

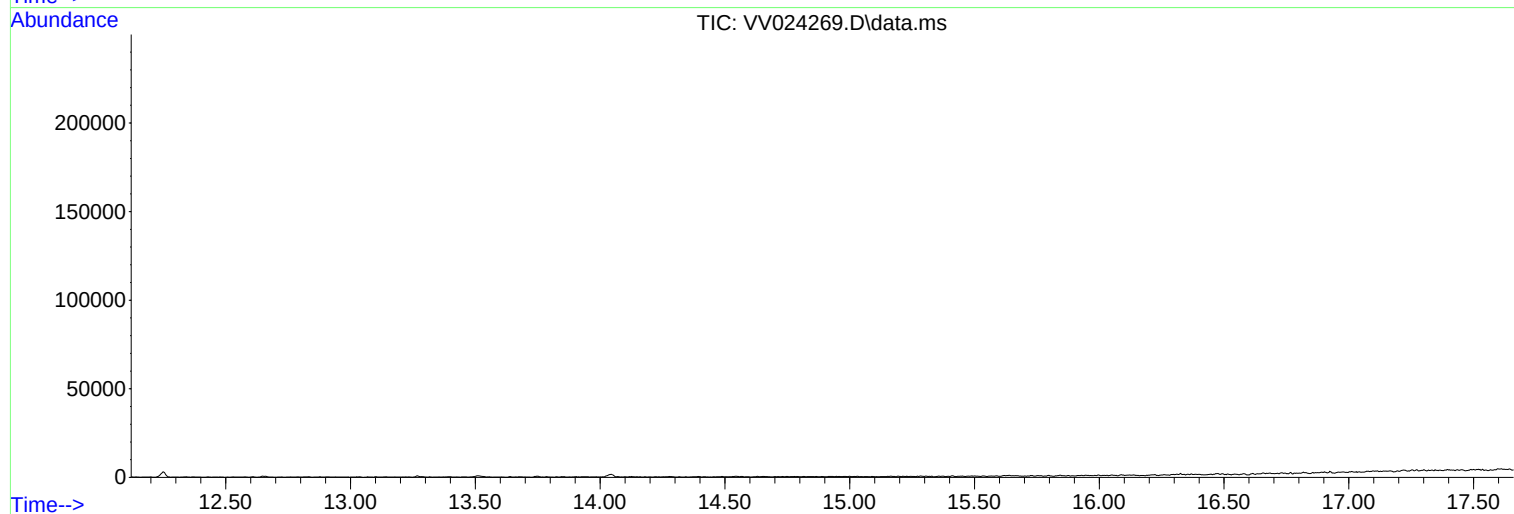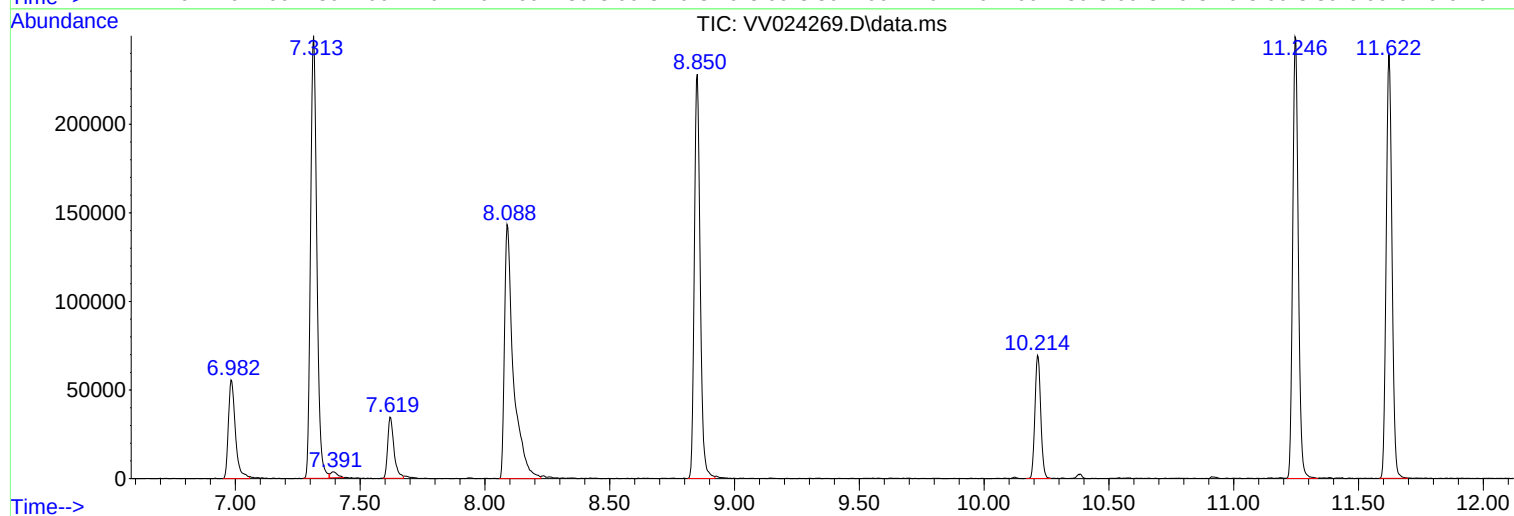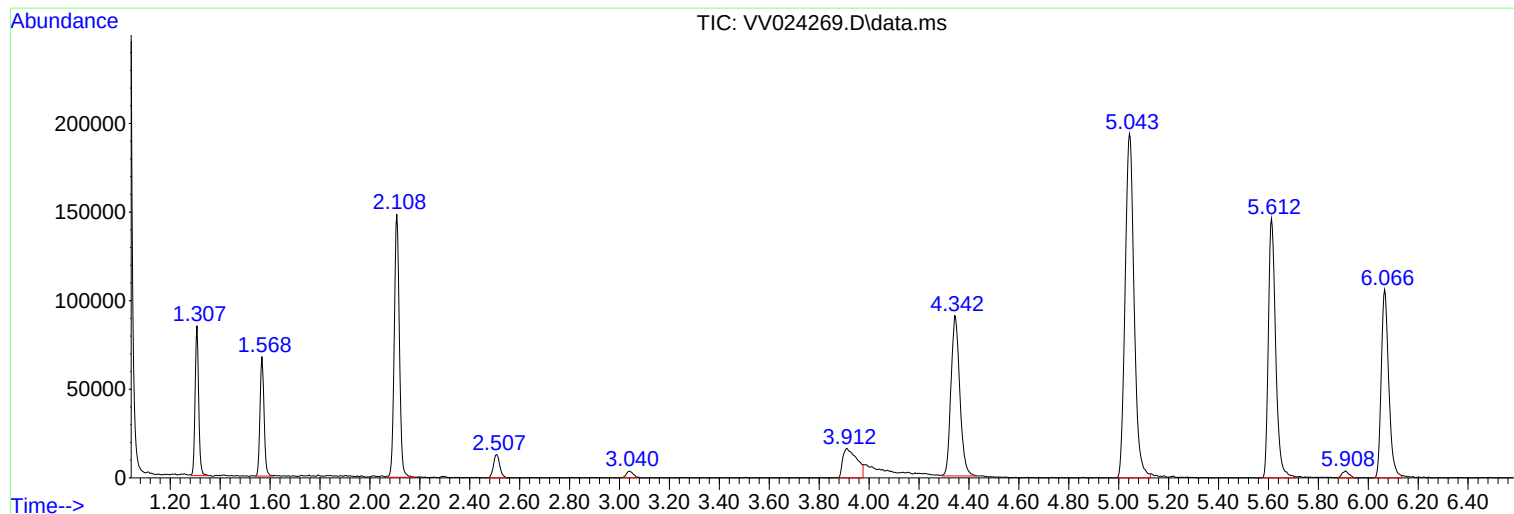

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
Data File : VV024269.D
Acq On : 04 Jan 2022 16:06
Operator : SY/MD
Sample : VV0104WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK287

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010422\
Data File : VV024269.D
Acq On : 04 Jan 2022 16:06
Operator : SY/MD
Sample : VV0104WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK287

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc