
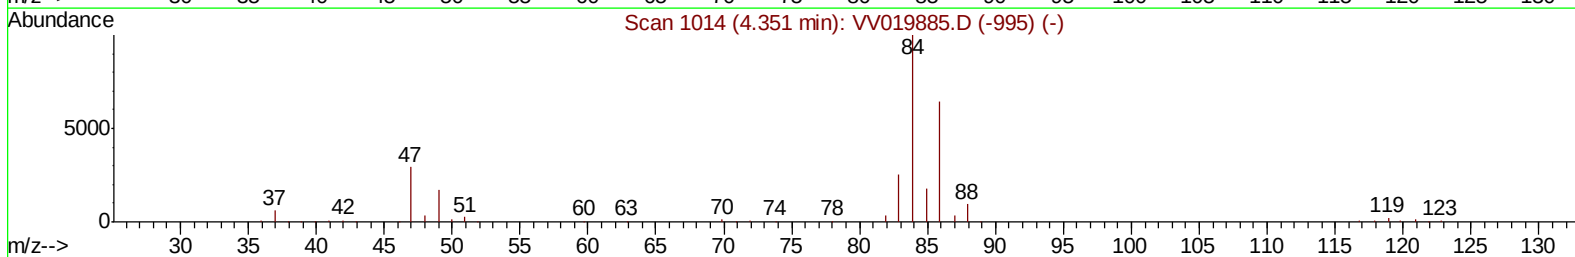
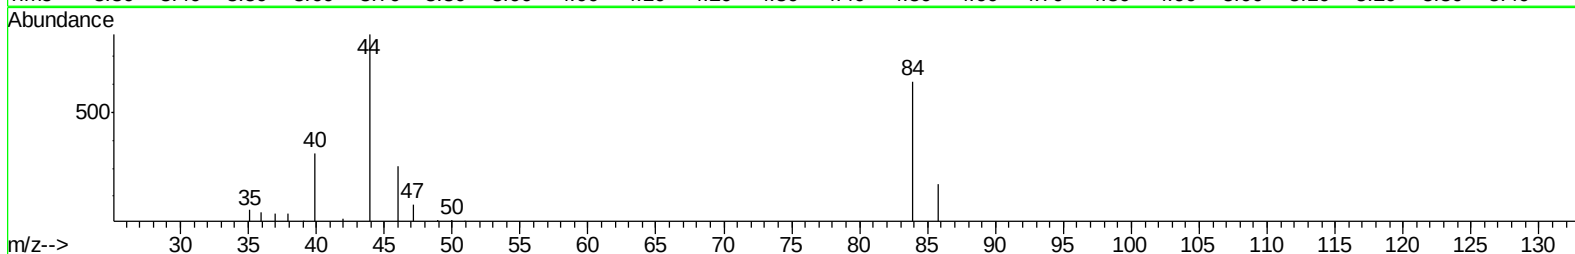


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019888.D
 Acq On : 05 Jan 2021 11:46
 Operator : SY/MD
 Sample : M1016-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 07:11:02 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 06 07:08:24 2021
 Response via : Initial Calibration

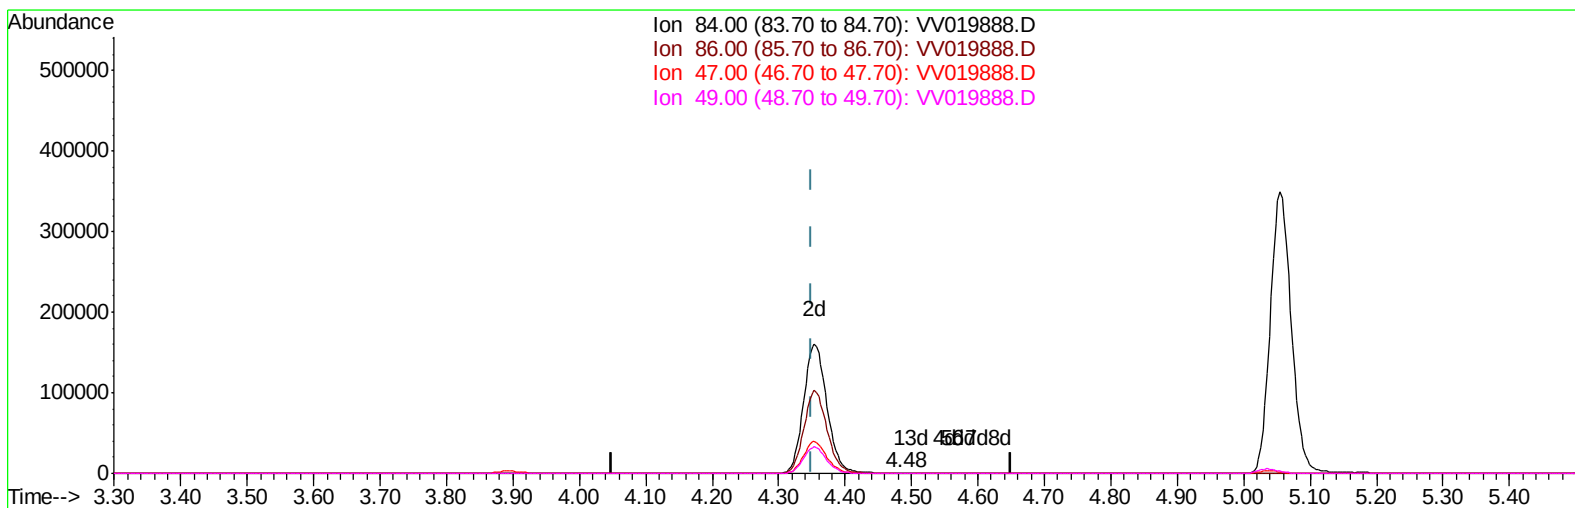

TIC: VV019888.D

(24) Chloroform-d (S)

4.482min (+0.132) 0.02ug/L

response 163

Ion	Exp%	Act%
84.00	100	100
86.00	61.60	51.53
47.00	46.50	58.28
49.00	28.00	28.22