
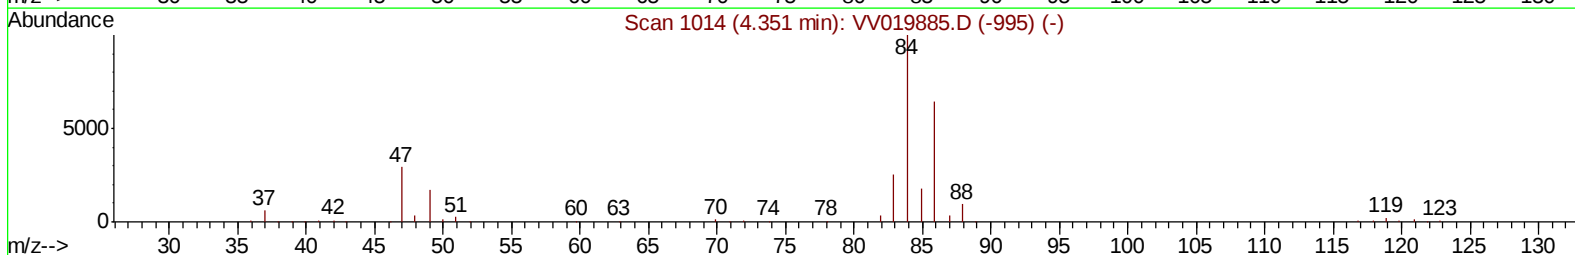
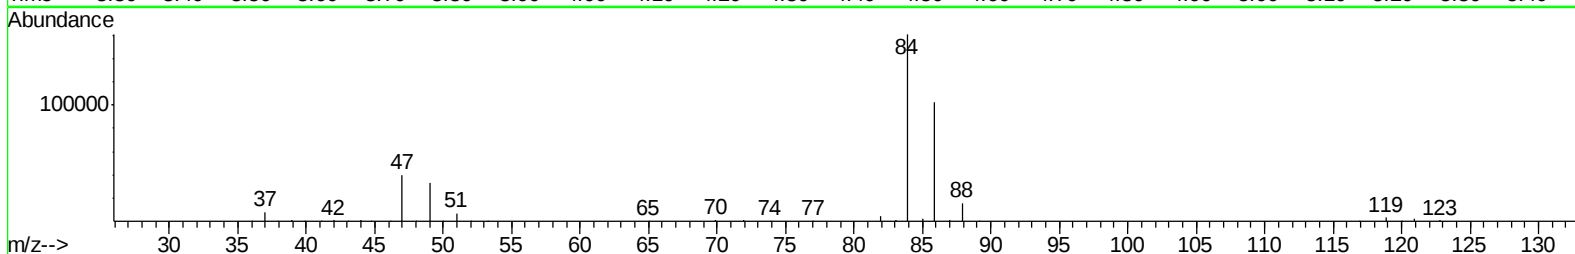


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\  
 Data File : VV019888.D  
 Acq On : 05 Jan 2021 11:46  
 Operator : SY/MD  
 Sample : M1016-02  
 Misc : 5.0mL/MSVOA V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 07:11:02 2021  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM122820WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Wed Jan 06 07:08:24 2021  
 Response via : Initial Calibration

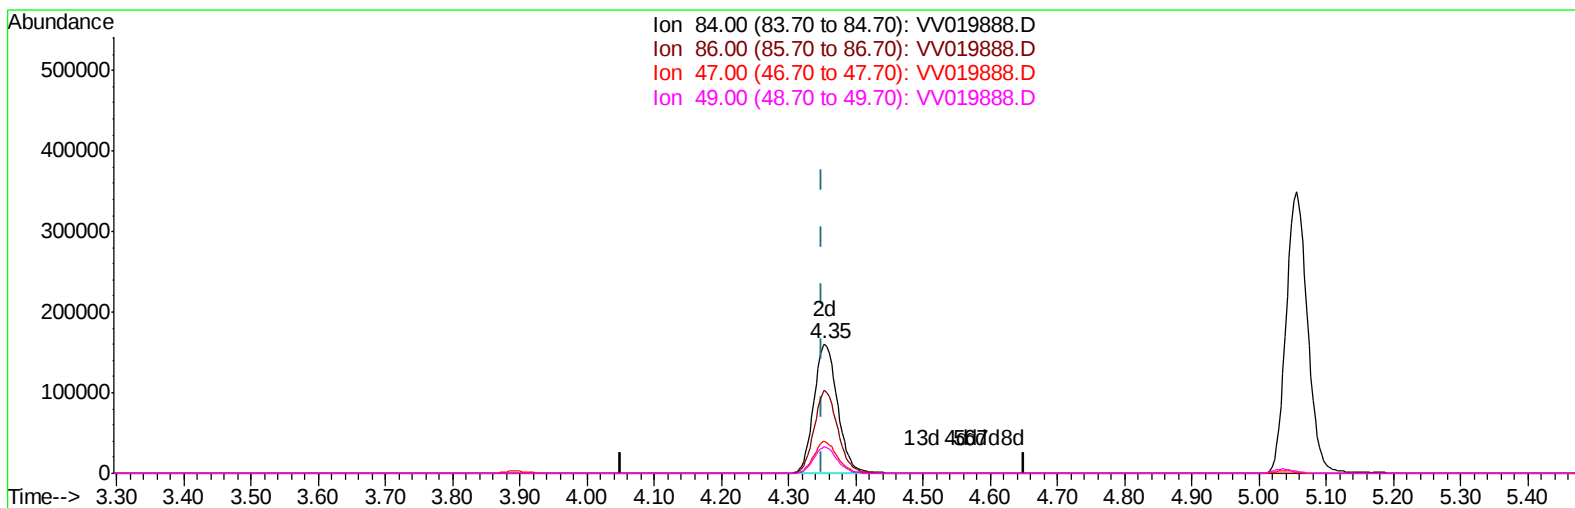

TIC: VV019888.D

(24) Chloroform-d (S)

4.354min (+0.003) 48.12ug/L m

response 393024

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 84.00 | 100   | 100   |
| 86.00 | 61.60 | 0.02# |
| 47.00 | 46.50 | 0.02# |
| 49.00 | 28.00 | 0.01# |