
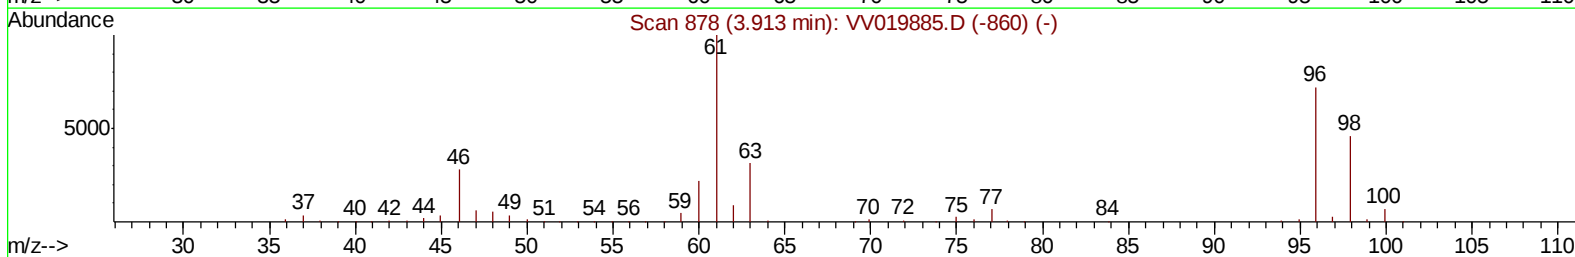
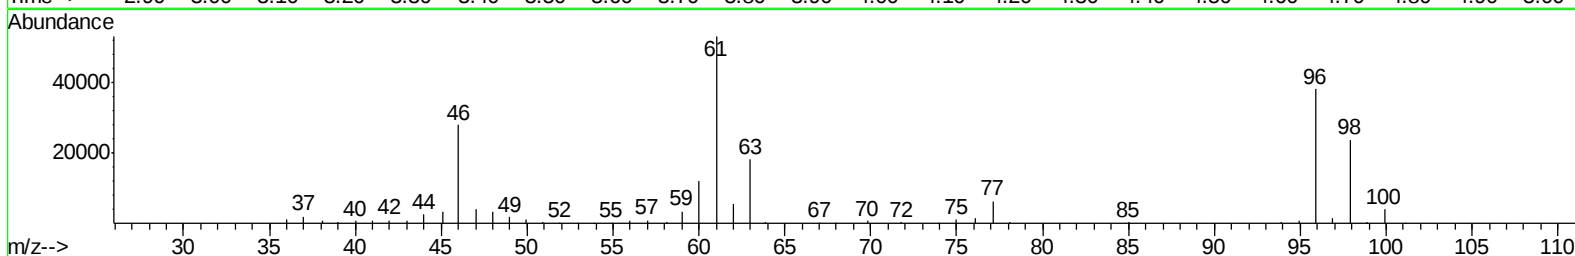


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019899.D
 Acq On : 05 Jan 2021 16:04
 Operator : SY/MD
 Sample : M1016-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 07:12:09 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 06 07:08:24 2021
 Response via : Initial Calibration

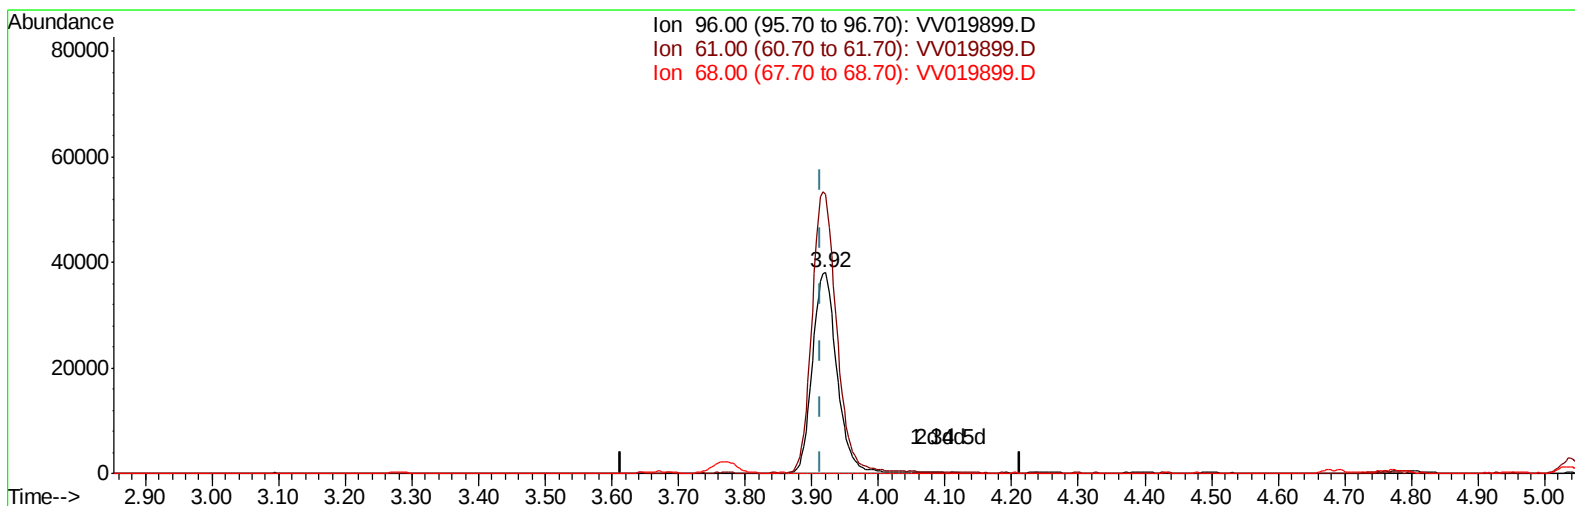

TIC: VV019899.D

(20) cis-1,2-Dichloroethene (T)

3.920min (+0.006) 23.58ug/L m

response 97934

Ion	Exp%	Act%
96.00	100	100
61.00	138.40	139.45
68.00	0.00	0.30#
0.00	0.00	0.00