

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019888.D
 Acq On : 05 Jan 2021 11:46
 Operator : SY/MD
 Sample : M1016-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Q7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	81	rVB	322104	327127	13.58%	1.826%
2	1.569	142	149	163	rBV	279768	317212	13.17%	1.771%
3	2.109	308	317	335	rBV	559020	840378	34.89%	4.692%
4	2.582	462	464	465	rBV	584	166	0.01%	0.001%
5	2.634	478	480	483	rBV2	624	426	0.02%	0.002%
6	2.817	533	537	539	rVB3	939	650	0.03%	0.004%
7	2.859	549	550	553	rBV4	617	227	0.01%	0.001%
8	2.891	557	560	563	rBV3	483	415	0.02%	0.002%
9	2.907	563	565	568	rBV2	848	573	0.02%	0.003%
10	3.090	621	622	625	rBV2	532	304	0.01%	0.002%
11	3.126	629	633	636	rBV4	657	429	0.02%	0.002%
12	3.138	636	637	639	rBV2	373	116	0.00%	0.001%
13	3.177	647	649	651	rBV4	752	340	0.01%	0.002%
14	3.244	667	670	674	rBV3	733	523	0.02%	0.003%
15	3.270	676	678	681	rBV3	569	302	0.01%	0.002%
16	3.322	692	694	695	rBV	543	174	0.01%	0.001%
17	3.347	700	702	706	rBV4	535	391	0.02%	0.002%
18	3.370	707	709	711	rBV2	540	249	0.01%	0.001%
19	3.392	714	716	718	rBV3	742	365	0.02%	0.002%
20	3.473	739	741	745	rBV3	666	453	0.02%	0.003%
21	3.489	745	746	749	rVB2	391	139	0.01%	0.001%
22	3.518	752	755	759	rVB4	916	588	0.02%	0.003%
23	3.537	759	761	762	rBV	421	222	0.01%	0.001%
24	3.543	762	763	764	rVV	468	100	0.00%	0.001%
25	3.611	782	784	787	rBV3	651	342	0.01%	0.002%
26	3.640	792	793	795	rVB2	567	161	0.01%	0.001%
27	3.679	802	805	809	rBV4	1023	961	0.04%	0.005%
28	3.704	812	813	814	rBV	389	113	0.00%	0.001%
29	3.749	819	827	828	rBV5	1505	1345	0.06%	0.008%
30	3.891	860	871	906	rBV	173279	507328	21.06%	2.832%
31	4.354	999	1015	1043	rBV	389873	951568	39.51%	5.313%
32	4.563	1075	1080	1083	rBV6	1544	1700	0.07%	0.009%
33	4.868	1171	1175	1180	rVB5	1183	1100	0.05%	0.006%
34	4.888	1180	1181	1182	rBV	439	145	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019888.D
 Acq On : 05 Jan 2021 11:46
 Operator : SY/MD
 Sample : M1016-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Q7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	4.904	1183	1186	1189	rBV3	726	510	0.02%	0.003%
36	4.961	1202	1204	1205	rBV2	657	283	0.01%	0.002%
37	5.051	1213	1232	1260	rBV2	933803	2408474	100.00%	13.447%
38	5.621	1396	1409	1440	rBV	693575	1398311	58.06%	7.807%
39	5.907	1487	1498	1519	rBV	59304	125833	5.22%	0.703%
40	6.074	1537	1550	1576	rBV	545074	1104999	45.88%	6.169%
41	6.421	1656	1658	1660	rBV3	750	344	0.01%	0.002%
42	6.453	1666	1668	1672	rVB2	903	473	0.02%	0.003%
43	6.514	1684	1687	1689	rBV2	712	393	0.02%	0.002%
44	6.852	1789	1792	1797	rVB5	935	785	0.03%	0.004%
45	6.884	1799	1802	1806	rBV4	836	749	0.03%	0.004%
46	6.913	1810	1811	1815	rVB3	638	233	0.01%	0.001%
47	6.936	1815	1818	1821	rBV3	1489	1017	0.04%	0.006%
48	6.990	1823	1835	1859	rBV	301995	549977	22.84%	3.071%
49	7.321	1924	1938	1961	rBV	1080151	1872893	77.76%	10.456%
50	7.627	2020	2033	2056	rBV	208909	367139	15.24%	2.050%
51	8.032	2156	2159	2160	rBV2	746	445	0.02%	0.002%
52	8.093	2167	2178	2216	rBV2	529888	1082407	44.94%	6.043%
53	8.440	2284	2286	2287	rBV	932	373	0.02%	0.002%
54	8.598	2331	2335	2337	rBV4	1336	1202	0.05%	0.007%
55	8.672	2355	2358	2361	rBV2	918	790	0.03%	0.004%
56	8.720	2371	2373	2374	rBV2	595	285	0.01%	0.002%
57	8.858	2403	2416	2446	rBV	1060882	1732186	71.92%	9.671%
58	9.074	2479	2483	2486	rBV4	1429	1127	0.05%	0.006%
59	9.244	2533	2536	2540	rBV3	1342	885	0.04%	0.005%
60	9.344	2565	2567	2568	rBV3	735	359	0.01%	0.002%
61	9.508	2615	2618	2620	rBV3	769	535	0.02%	0.003%
62	10.016	2772	2776	2778	rBV2	1394	1110	0.05%	0.006%
63	10.154	2813	2819	2822	rBV7	1439	1251	0.05%	0.007%
64	10.222	2828	2840	2861	rBV	607193	960989	39.90%	5.365%
65	10.389	2885	2892	2900	rVB6	5879	7725	0.32%	0.043%
66	10.518	2929	2932	2935	rBV3	991	843	0.04%	0.005%
67	10.736	2998	3000	3001	rBV2	539	186	0.01%	0.001%
68	10.788	3014	3016	3020	rVB3	1012	533	0.02%	0.003%
69	10.980	3074	3076	3078	rBV2	773	374	0.02%	0.002%
70	11.064	3099	3102	3104	rBV3	1419	688	0.03%	0.004%
71	11.164	3131	3133	3136	rBV4	1049	842	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019888.D
 Acq On : 05 Jan 2021 11:46
 Operator : SY/MD
 Sample : M1016-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Q7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	11.257	3148	3162	3181	rBV	1048037	1633753	67.83%	9.121%
73	11.482	3230	3232	3234	rBV3	842	345	0.01%	0.002%
74	11.633	3267	3279	3303	rBV	1088792	1688285	70.10%	9.426%
75	11.855	3344	3348	3349	rBV2	767	493	0.02%	0.003%
76	12.019	3396	3399	3402	rBV3	732	507	0.02%	0.003%
77	12.196	3450	3454	3455	rBV2	809	486	0.02%	0.003%
78	12.514	3551	3553	3557	rBV3	803	596	0.02%	0.003%
79	12.726	3614	3619	3622	rBV5	1225	1014	0.04%	0.006%
80	12.742	3622	3624	3627	rVV3	817	470	0.02%	0.003%
81	13.440	3839	3841	3844	rBV3	999	695	0.03%	0.004%
82	14.128	4052	4055	4057	rBV3	957	531	0.02%	0.003%


Sum of corrected areas: 17911355

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010521\
Data File : VV019888.D
Acq On : 05 Jan 2021 11:46
Operator : SY/MD
Sample : M1016-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Q7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

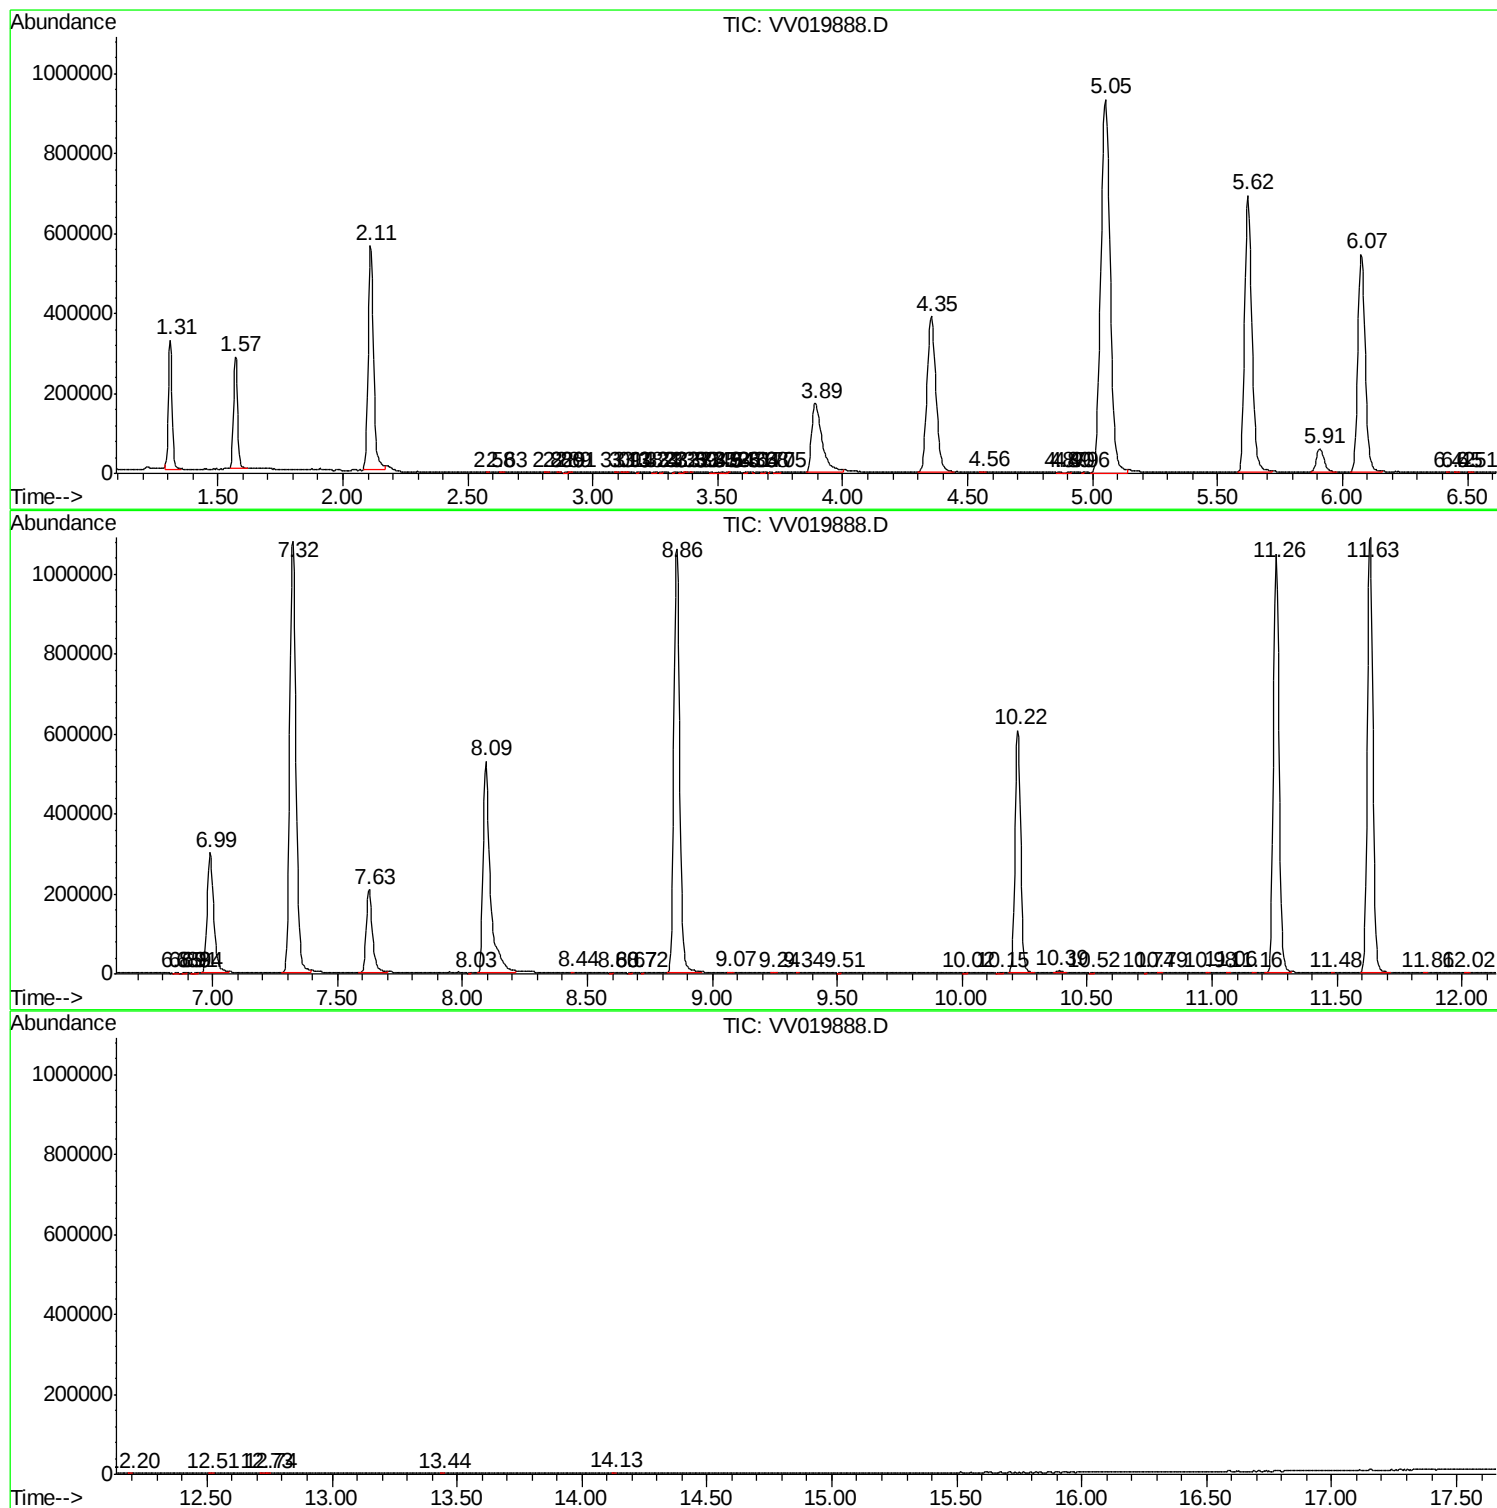

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010521\
Data File : VV019888.D
Acq On : 05 Jan 2021 11:46
Operator : SY/MD
Sample : M1016-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Q7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV010521\
Data File : VV019888.D
Acq On : 05 Jan 2021 11:46
Operator : SY/MD
Sample : M1016-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Q7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc