

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019889.D
 Acq On : 05 Jan 2021 12:09
 Operator : SY/MD
 Sample : M1017-01 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	82	rVB	329236	326162	1.92%	0.857%
2	1.569	143	149	163	rVB	279770	316617	1.86%	0.832%
3	2.110	308	317	350	rVB	567008	881975	5.18%	2.317%
4	2.714	501	505	508	rBV4	633	626	0.00%	0.002%
5	2.875	553	555	556	rBV	1057	442	0.00%	0.001%
6	2.936	572	574	576	rBV2	644	205	0.00%	0.001%
7	3.126	628	633	634	rBV3	981	866	0.01%	0.002%
8	3.151	639	641	644	rBV3	528	315	0.00%	0.001%
9	3.193	652	654	656	rVB3	496	169	0.00%	0.000%
10	3.251	668	672	675	rBV3	1045	856	0.01%	0.002%
11	3.277	677	680	683	rVV4	514	397	0.00%	0.001%
12	3.322	690	694	698	rBV5	979	824	0.00%	0.002%
13	3.408	719	721	724	rVB3	829	415	0.00%	0.001%
14	3.431	724	728	731	rBV4	716	557	0.00%	0.001%
15	3.447	731	733	736	rVB2	1135	588	0.00%	0.002%
16	3.470	736	740	741	rBV2	631	449	0.00%	0.001%
17	3.521	752	756	758	rBV3	543	292	0.00%	0.001%
18	3.534	758	760	767	rVB6	1241	1414	0.01%	0.004%
19	3.560	767	768	770	rBV2	229	62	0.00%	0.000%
20	3.579	770	774	776	rBV2	699	610	0.00%	0.002%
21	3.624	786	788	792	rVB3	846	587	0.00%	0.002%
22	3.643	792	794	797	rBV2	371	240	0.00%	0.001%
23	3.675	802	804	807	rBV2	512	349	0.00%	0.001%
24	3.704	812	813	814	rVB	680	131	0.00%	0.000%
25	3.724	816	819	827	rBV4	899	940	0.01%	0.002%
26	3.762	827	831	832	rBV3	738	524	0.00%	0.001%
27	3.894	861	872	917	rBV	173697	596181	3.50%	1.566%
28	4.354	999	1015	1043	rBV	391045	957391	5.63%	2.515%
29	4.679	1112	1116	1118	rBV3	766	575	0.00%	0.002%
30	4.707	1123	1125	1129	rVB5	1386	883	0.01%	0.002%
31	4.733	1129	1133	1134	rBV2	592	429	0.00%	0.001%
32	4.759	1139	1141	1146	rBV4	536	522	0.00%	0.001%
33	4.810	1150	1157	1158	rVB2	619	679	0.00%	0.002%
34	4.830	1158	1163	1167	rBV6	1247	1446	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019889.D
 Acq On : 05 Jan 2021 12:09
 Operator : SY/MD
 Sample : M1017-01 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	4.888	1179	1181	1184	rBV4	898	498	0.00%	0.001%
36	5.051	1214	1232	1273	rBV2	931709	2468951	14.51%	6.485%
37	5.482	1364	1366	1367	rBV2	782	251	0.00%	0.001%
38	5.621	1397	1409	1439	rBV	708928	1417773	8.33%	3.724%
39	5.920	1487	1502	1525	rBV	1468899	2882741	16.94%	7.572%
40	6.074	1538	1550	1570	rBV	539908	1087280	6.39%	2.856%
41	6.415	1654	1656	1658	rBV3	591	301	0.00%	0.001%
42	6.437	1658	1663	1664	rBV4	870	675	0.00%	0.002%
43	6.585	1707	1709	1710	rBV2	444	168	0.00%	0.000%
44	6.752	1759	1761	1763	rBV3	591	345	0.00%	0.001%
45	6.871	1793	1798	1801	rBV4	1139	1191	0.01%	0.003%
46	6.945	1819	1821	1823	rBV2	513	284	0.00%	0.001%
47	6.990	1823	1835	1860	rVV	307704	554197	3.26%	1.456%
48	7.322	1925	1938	1962	rBV	1087167	1877236	11.03%	4.931%
49	7.550	2007	2009	2011	rBV2	1252	449	0.00%	0.001%
50	7.627	2023	2033	2055	rBV	206452	364812	2.14%	0.958%
51	7.981	2128	2143	2168	rBV	10311474	17014694	100.00%	44.694%
52	8.093	2169	2178	2212	rVB2	581384	1121608	6.59%	2.946%
53	8.691	2360	2364	2367	rBV3	1353	1007	0.01%	0.003%
54	8.717	2367	2372	2375	rVV6	788	740	0.00%	0.002%
55	8.797	2395	2397	2400	rVB2	716	270	0.00%	0.001%
56	8.858	2404	2416	2439	rBV	1084229	1752131	10.30%	4.602%
57	9.280	2544	2547	2548	rBV2	933	541	0.00%	0.001%
58	9.302	2552	2554	2556	rBV3	820	384	0.00%	0.001%
59	9.328	2561	2562	2563	rBV3	301	116	0.00%	0.000%
60	9.341	2563	2566	2567	rBV3	755	386	0.00%	0.001%
61	9.546	2626	2630	2631	rBV3	1407	861	0.01%	0.002%
62	9.640	2657	2659	2662	rBV4	704	257	0.00%	0.001%
63	9.720	2682	2684	2685	rBV3	661	262	0.00%	0.001%
64	9.778	2696	2702	2704	rBV3	1001	810	0.00%	0.002%
65	9.820	2713	2715	2717	rBV2	636	428	0.00%	0.001%
66	9.939	2749	2752	2757	rBV3	1049	865	0.01%	0.002%
67	9.971	2760	2762	2763	rBV	987	418	0.00%	0.001%
68	10.000	2769	2771	2773	rBV2	545	303	0.00%	0.001%
69	10.096	2797	2801	2802	rBV2	1004	542	0.00%	0.001%
70	10.141	2811	2815	2819	rBV5	819	768	0.00%	0.002%
71	10.222	2828	2840	2863	rVB	663071	1037696	6.10%	2.726%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019889.D
 Acq On : 05 Jan 2021 12:09
 Operator : SY/MD
 Sample : M1017-01 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.582	2950	2952	2959	rVB5	877	823	0.00%	0.002%
73	10.640	2967	2970	2973	rBV3	1015	642	0.00%	0.002%
74	10.739	2999	3001	3002	rBV2	752	318	0.00%	0.001%
75	10.794	3015	3018	3020	rBV3	602	273	0.00%	0.001%
76	10.910	3050	3054	3056	rBV3	1010	720	0.00%	0.002%
77	10.971	3070	3073	3078	rVB2	834	558	0.00%	0.001%
78	11.071	3102	3104	3107	rBV3	1035	593	0.00%	0.002%
79	11.128	3119	3122	3123	rBV2	608	332	0.00%	0.001%
80	11.177	3134	3137	3141	rBV5	1300	1116	0.01%	0.003%
81	11.257	3150	3162	3186	rBV	1083193	1669112	9.81%	4.384%
82	11.630	3266	3278	3299	rBV	1072870	1701974	10.00%	4.471%
83	11.826	3335	3339	3342	rBV3	974	790	0.00%	0.002%
84	11.845	3342	3345	3347	rBV4	1064	846	0.00%	0.002%
85	12.013	3395	3397	3400	rBV2	1051	712	0.00%	0.002%
86	12.074	3413	3416	3418	rBV3	1026	721	0.00%	0.002%
87	12.456	3533	3535	3537	rVB2	686	240	0.00%	0.001%
88	12.861	3659	3661	3664	rBV4	1055	637	0.00%	0.002%
89	12.939	3683	3685	3690	rVB5	1410	1201	0.01%	0.003%
90	13.627	3896	3899	3901	rBV3	1027	873	0.01%	0.002%


Sum of corrected areas: 38069438

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010521\
Data File : VV019889.D
Acq On : 05 Jan 2021 12:09
Operator : SY/MD
Sample : M1017-01 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

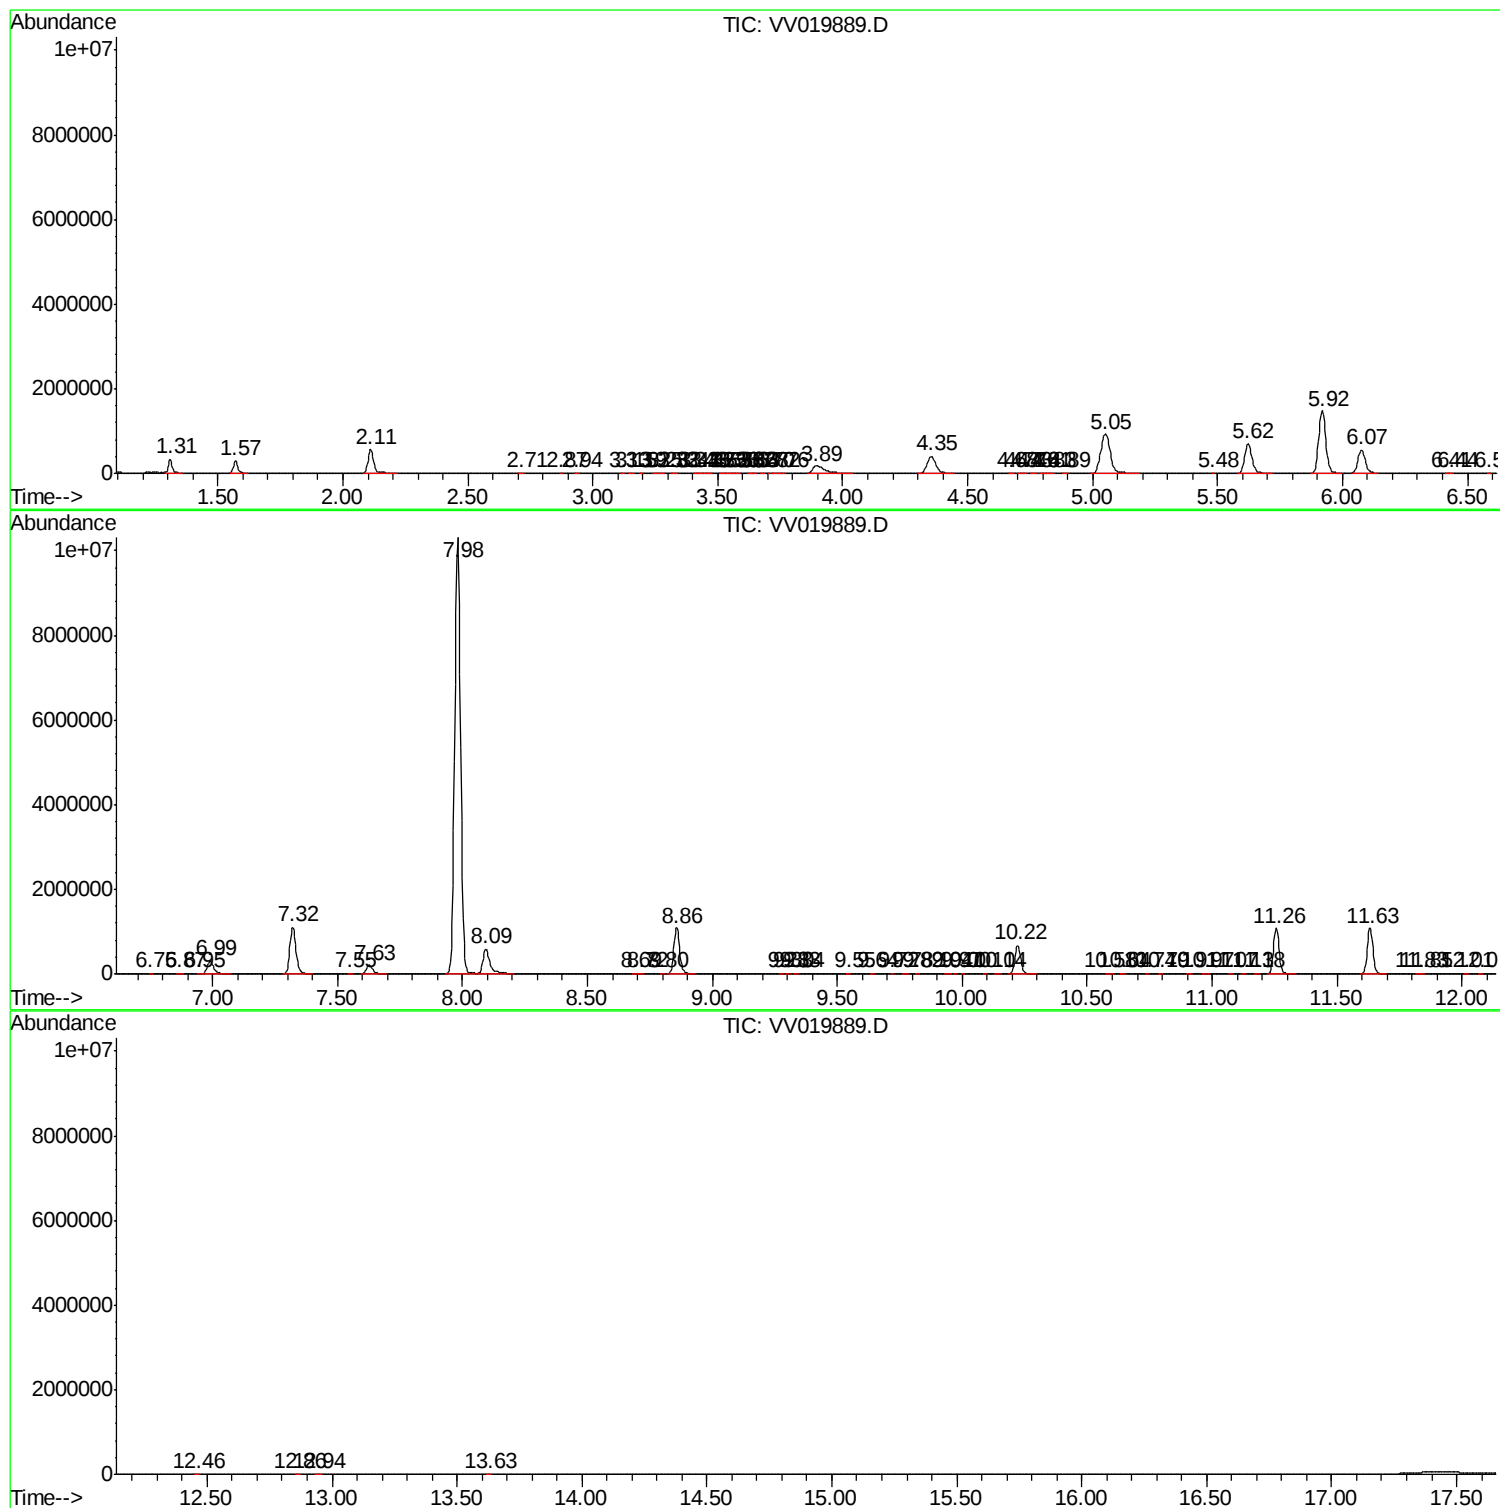

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010521\
Data File : VV019889.D
Acq On : 05 Jan 2021 12:09
Operator : SY/MD
Sample : M1017-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV010521\
Data File : VV019889.D
Acq On : 05 Jan 2021 12:09
Operator : SY/MD
Sample : M1017-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc