

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019890.D
 Acq On : 05 Jan 2021 12:33
 Operator : SY/MD
 Sample : M1017-02 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	86	rVB	318941	324794	13.30%	1.740%
2	1.569	142	149	165	rVB	277521	312892	12.81%	1.676%
3	2.110	308	317	345	rVB	562461	856389	35.06%	4.587%
4	2.730	508	510	512	rBV3	691	338	0.01%	0.002%
5	2.875	551	555	557	rBV3	708	652	0.03%	0.003%
6	2.929	568	572	575	rVB2	1043	803	0.03%	0.004%
7	2.952	575	579	581	rBV3	827	732	0.03%	0.004%
8	2.994	590	592	594	rVB2	725	302	0.01%	0.002%
9	3.010	594	597	599	rVB3	813	332	0.01%	0.002%
10	3.023	599	601	602	rBV	996	487	0.02%	0.003%
11	3.116	628	630	635	rVB7	1158	725	0.03%	0.004%
12	3.145	636	639	642	rVB4	722	537	0.02%	0.003%
13	3.164	642	645	649	rBV4	558	491	0.02%	0.003%
14	3.203	655	657	659	rBV2	868	461	0.02%	0.002%
15	3.322	688	694	696	rBV3	925	870	0.04%	0.005%
16	3.396	715	717	720	rVB3	709	312	0.01%	0.002%
17	3.463	735	738	740	rBV2	549	320	0.01%	0.002%
18	3.553	764	766	770	rBV3	406	253	0.01%	0.001%
19	3.682	805	806	808	rBV2	448	161	0.01%	0.001%
20	3.695	808	810	811	rBV	776	286	0.01%	0.002%
21	3.737	819	823	828	rBV5	907	1142	0.05%	0.006%
22	3.756	828	829	833	rVB2	995	479	0.02%	0.003%
23	3.775	833	835	838	rVB3	998	422	0.02%	0.002%
24	3.794	838	841	842	rBV	514	271	0.01%	0.001%
25	3.817	846	848	850	rBV	761	306	0.01%	0.002%
26	3.839	850	855	856	rBV4	1246	966	0.04%	0.005%
27	3.897	861	873	908	rBV	176236	561617	22.99%	3.008%
28	4.354	1001	1015	1040	rVB	391111	947335	38.78%	5.074%
29	4.782	1146	1148	1149	rVB2	571	162	0.01%	0.001%
30	5.052	1213	1232	1260	rBV2	951260	2442664	100.00%	13.084%
31	5.470	1359	1362	1364	rBV2	1135	907	0.04%	0.005%
32	5.553	1383	1388	1390	rBV3	973	1026	0.04%	0.005%
33	5.621	1396	1409	1438	rBV	715121	1430063	58.55%	7.660%
34	5.913	1487	1500	1516	rBV6	55621	127423	5.22%	0.683%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019890.D
 Acq On : 05 Jan 2021 12:33
 Operator : SY/MD
 Sample : M1017-02 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	6.074	1536	1550	1573	rBV	551853	1121457	45.91%	6.007%
36	6.341	1631	1633	1635	rBV2	578	307	0.01%	0.002%
37	6.370	1640	1642	1644	rBV2	924	488	0.02%	0.003%
38	6.396	1648	1650	1651	rBV2	980	452	0.02%	0.002%
39	6.540	1692	1695	1696	rBV3	592	276	0.01%	0.001%
40	6.617	1717	1719	1720	rBV2	1313	555	0.02%	0.003%
41	6.826	1781	1784	1786	rBV3	799	523	0.02%	0.003%
42	6.894	1803	1805	1806	rBV	378	177	0.01%	0.001%
43	6.907	1806	1809	1810	rVV3	771	351	0.01%	0.002%
44	6.926	1813	1815	1819	rBV3	639	530	0.02%	0.003%
45	6.990	1823	1835	1860	rBV	303273	550319	22.53%	2.948%
46	7.322	1926	1938	1965	rBV	1092034	1874990	76.76%	10.043%
47	7.627	2022	2033	2060	rBV	210464	369188	15.11%	1.978%
48	7.933	2124	2128	2129	rBV3	817	560	0.02%	0.003%
49	7.981	2130	2143	2159	rBV	251907	429236	17.57%	2.299%
50	8.093	2168	2178	2210	rBV2	576768	1125449	46.07%	6.028%
51	8.855	2401	2415	2443	rBV	1075600	1763121	72.18%	9.444%
52	9.235	2530	2533	2535	rBV3	729	465	0.02%	0.002%
53	9.328	2559	2562	2563	rBV2	867	442	0.02%	0.002%
54	9.440	2592	2597	2600	rVB4	1457	1251	0.05%	0.007%
55	9.453	2600	2601	2602	rBV4	521	187	0.01%	0.001%
56	9.582	2638	2641	2643	rBV3	1384	855	0.04%	0.005%
57	9.604	2646	2648	2650	rBV3	786	429	0.02%	0.002%
58	9.691	2673	2675	2678	rBV3	614	417	0.02%	0.002%
59	9.736	2685	2689	2691	rBV3	937	747	0.03%	0.004%
60	9.791	2703	2706	2709	rBV3	601	490	0.02%	0.003%
61	9.813	2709	2713	2717	rBV3	1078	819	0.03%	0.004%
62	9.903	2737	2741	2747	rBV6	1416	1607	0.07%	0.009%
63	9.929	2747	2749	2752	rBV3	531	333	0.01%	0.002%
64	10.135	2810	2813	2816	rBV4	453	319	0.01%	0.002%
65	10.222	2828	2840	2863	rBV	663194	1036799	42.45%	5.554%
66	10.666	2974	2978	2980	rBV2	1076	802	0.03%	0.004%
67	10.688	2983	2985	2986	rBV2	403	162	0.01%	0.001%
68	10.781	3012	3014	3019	rVB4	1098	647	0.03%	0.003%
69	10.903	3049	3052	3054	rBV2	998	718	0.03%	0.004%
70	11.058	3098	3100	3102	rVB2	737	283	0.01%	0.002%
71	11.080	3102	3107	3109	rBV4	814	563	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
Data File : VV019890.D
Acq On : 05 Jan 2021 12:33
Operator : SY/MD
Sample : M1017-02 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Title : VOC Analysis

72	11.145	3125	3127	3128	rBV2	746	267	0.01%	0.001%
73	11.257	3149	3162	3181	rBV	1064931	1658271	67.89%	8.883%
74	11.530	3245	3247	3249	rBV2	777	491	0.02%	0.003%
75	11.630	3266	3278	3296	rBV	1074573	1699074	69.56%	9.101%
76	12.019	3397	3399	3403	rBV4	1093	741	0.03%	0.004%
77	12.199	3452	3455	3462	rBV5	1292	1781	0.07%	0.010%
78	12.530	3554	3558	3563	rBV6	915	837	0.03%	0.004%
79	12.611	3580	3583	3590	rBV4	953	997	0.04%	0.005%
80	12.640	3590	3592	3594	rBV	1167	616	0.03%	0.003%
81	13.315	3798	3802	3805	rBV3	1170	1338	0.05%	0.007%
82	13.402	3827	3829	3830	rBV	724	266	0.01%	0.001%
83	13.730	3927	3931	3934	rBV4	954	895	0.04%	0.005%


Sum of corrected areas: 18668808

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010521\
Data File : VV019890.D
Acq On : 05 Jan 2021 12:33
Operator : SY/MD
Sample : M1017-02 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

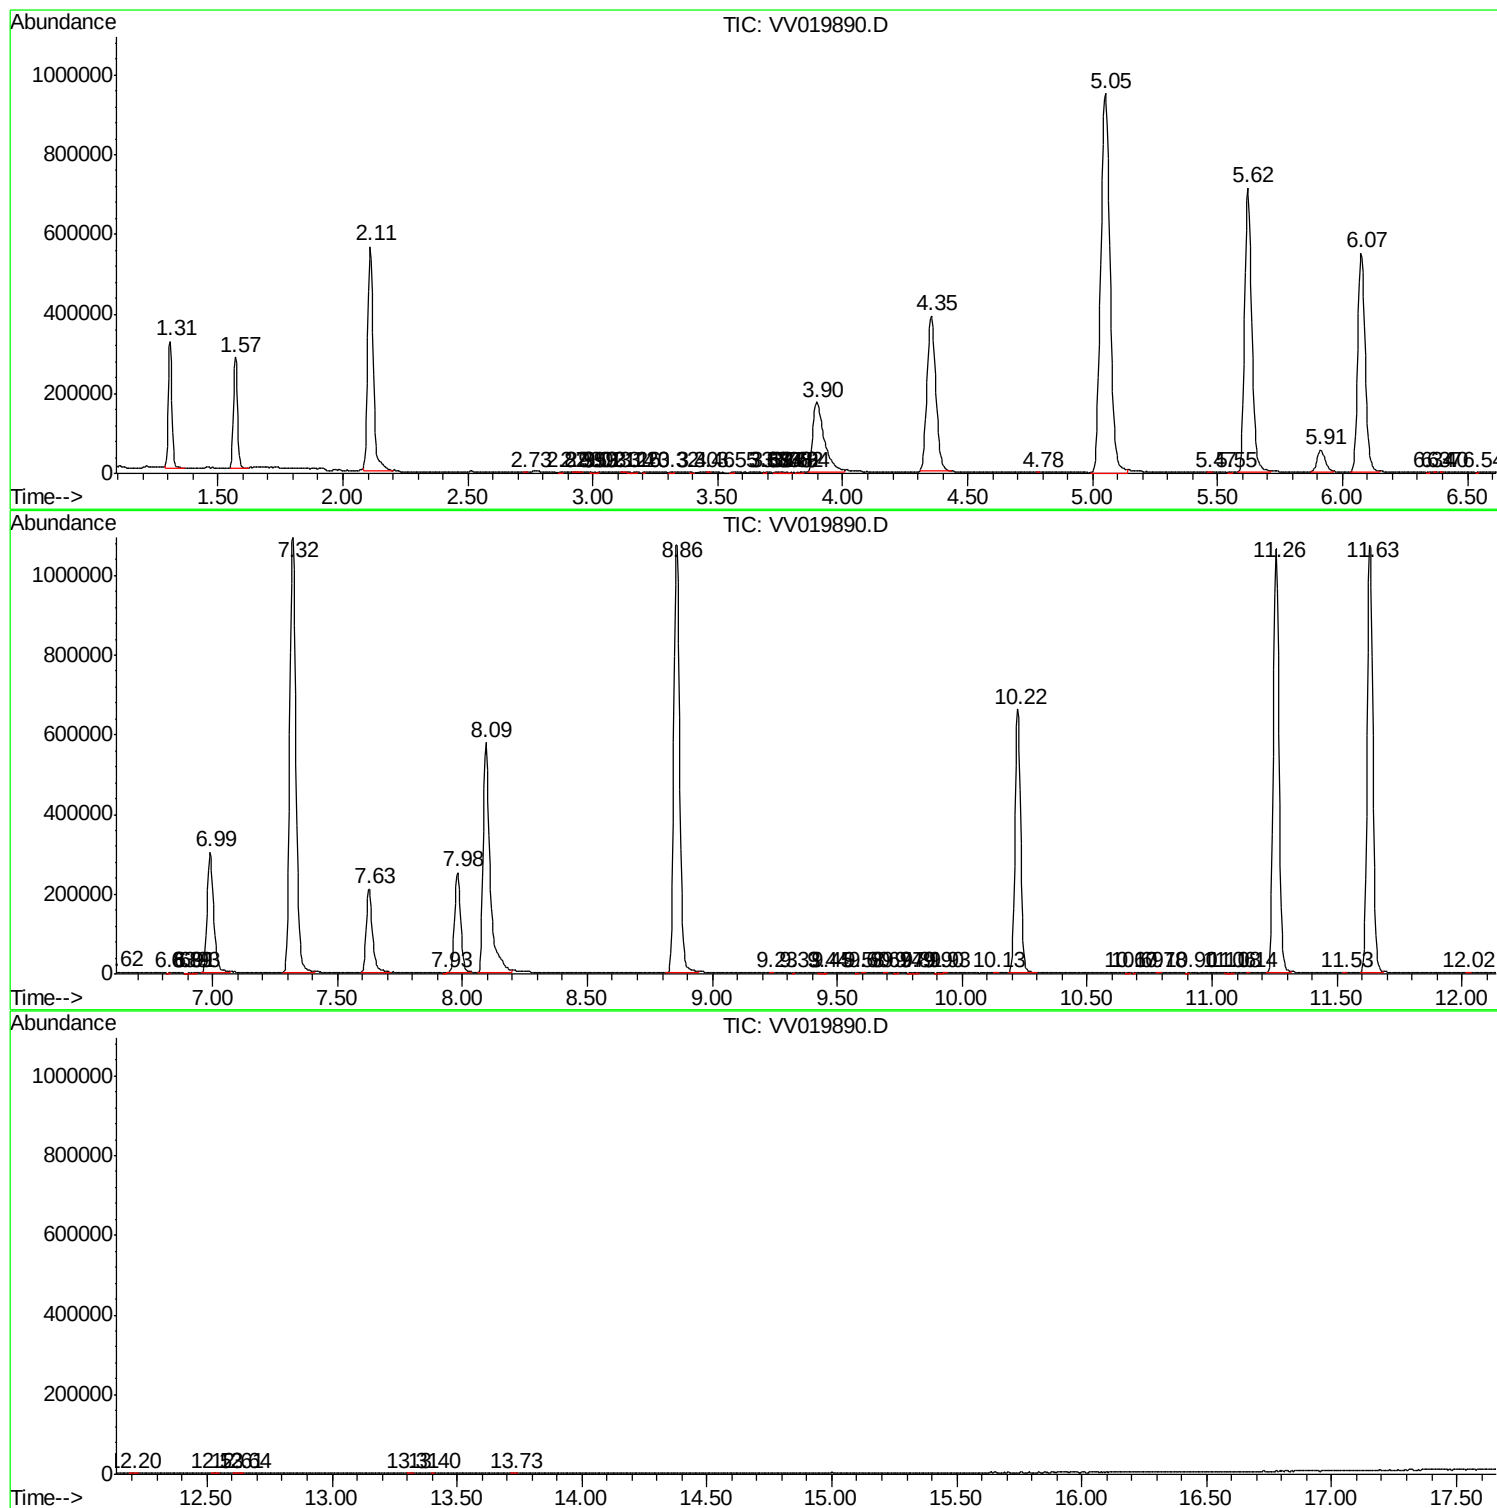

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010521\
Data File : VV019890.D
Acq On : 05 Jan 2021 12:33
Operator : SY/MD
Sample : M1017-02 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010521\
Data File : VV019890.D
Acq On : 05 Jan 2021 12:33
Operator : SY/MD
Sample : M1017-02 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4W3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc