

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019894.D
 Acq On : 05 Jan 2021 14:07
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	86	rVB	326669	324894	13.96%	1.836%
2	1.569	142	149	164	rVB	268220	303884	13.06%	1.717%
3	2.110	308	317	344	rVB	533647	804582	34.57%	4.547%
4	2.820	536	538	540	rBV3	746	393	0.02%	0.002%
5	2.962	578	582	584	rBV4	929	764	0.03%	0.004%
6	3.010	595	597	600	rVB2	914	451	0.02%	0.003%
7	3.036	602	605	607	rVV3	1017	666	0.03%	0.004%
8	3.074	611	617	620	rBV5	1173	1281	0.06%	0.007%
9	3.122	630	632	633	rBV2	637	287	0.01%	0.002%
10	3.180	649	650	653	rBV3	514	365	0.02%	0.002%
11	3.270	677	678	681	rBV2	403	271	0.01%	0.002%
12	3.306	687	689	692	rVB4	728	375	0.02%	0.002%
13	3.393	712	716	718	rBV2	843	517	0.02%	0.003%
14	3.415	721	723	724	rBV	480	131	0.01%	0.001%
15	3.547	762	764	765	rBV	331	150	0.01%	0.001%
16	3.557	765	767	770	rVB3	986	485	0.02%	0.003%
17	3.576	770	773	776	rBV2	718	448	0.02%	0.003%
18	3.598	776	780	784	rBV6	815	821	0.04%	0.005%
19	3.640	790	793	794	rBV3	585	344	0.01%	0.002%
20	3.698	808	811	812	rBV3	776	416	0.02%	0.002%
21	3.778	832	836	838	rBV3	737	503	0.02%	0.003%
22	3.823	849	850	852	rBV	692	273	0.01%	0.002%
23	3.894	861	872	909	rBV	173133	549226	23.60%	3.104%
24	4.354	1000	1015	1043	rBV	374676	918353	39.46%	5.190%
25	4.663	1109	1111	1114	rBV3	884	581	0.02%	0.003%
26	4.817	1157	1159	1163	rVB3	1236	688	0.03%	0.004%
27	4.836	1163	1165	1168	rBV2	960	666	0.03%	0.004%
28	4.878	1175	1178	1179	rBV2	486	225	0.01%	0.001%
29	4.901	1179	1185	1187	rVV5	526	471	0.02%	0.003%
30	5.052	1214	1232	1261	rBV2	914395	2327591	100.00%	13.154%
31	5.531	1379	1381	1384	rVB3	969	344	0.01%	0.002%
32	5.621	1394	1409	1442	rBV	710467	1428221	61.36%	8.071%
33	5.910	1490	1499	1514	rVB2	40473	77867	3.35%	0.440%
34	6.074	1537	1550	1573	rBV	528932	1063745	45.70%	6.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019894.D
 Acq On : 05 Jan 2021 14:07
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	6.418	1652	1657	1660	rBV5	1477	1686	0.07%	0.010%
36	6.450	1664	1667	1669	rBV3	846	488	0.02%	0.003%
37	6.556	1697	1700	1703	rVB4	918	662	0.03%	0.004%
38	6.576	1703	1706	1708	rBV3	500	353	0.02%	0.002%
39	6.589	1708	1710	1713	rVB3	964	504	0.02%	0.003%
40	6.611	1715	1717	1719	rBV3	746	333	0.01%	0.002%
41	6.675	1735	1737	1741	rBV3	899	654	0.03%	0.004%
42	6.775	1766	1768	1769	rBV	534	231	0.01%	0.001%
43	6.836	1786	1787	1789	rBV2	491	243	0.01%	0.001%
44	6.849	1789	1791	1794	rVB3	1111	638	0.03%	0.004%
45	6.897	1803	1806	1807	rBV3	566	203	0.01%	0.001%
46	6.942	1817	1820	1821	rBV2	672	478	0.02%	0.003%
47	6.990	1824	1835	1860	rVV	286557	523626	22.50%	2.959%
48	7.318	1924	1937	1966	rBV	1021268	1776763	76.33%	10.041%
49	7.627	2022	2033	2058	rBV2	196320	351531	15.10%	1.987%
50	7.984	2135	2144	2157	rVB7	9355	17440	0.75%	0.099%
51	8.093	2168	2178	2214	rBV2	579852	1134149	48.73%	6.409%
52	8.614	2338	2340	2341	rBV2	643	223	0.01%	0.001%
53	8.701	2364	2367	2369	rBV3	960	597	0.03%	0.003%
54	8.791	2393	2395	2398	rBV3	830	654	0.03%	0.004%
55	8.855	2403	2415	2446	rBV	1062738	1749787	75.18%	9.889%
56	9.196	2518	2521	2526	rBV5	796	918	0.04%	0.005%
57	9.367	2571	2574	2576	rBV3	606	353	0.02%	0.002%
58	9.376	2576	2577	2580	rVB2	1156	444	0.02%	0.003%
59	9.399	2580	2584	2585	rBV4	730	502	0.02%	0.003%
60	9.495	2611	2614	2615	rBV2	821	564	0.02%	0.003%
61	9.553	2630	2632	2633	rBV2	488	200	0.01%	0.001%
62	9.630	2653	2656	2658	rBV4	633	360	0.02%	0.002%
63	9.646	2658	2661	2664	rVV3	944	723	0.03%	0.004%
64	9.894	2731	2738	2739	rBV5	1136	1038	0.04%	0.006%
65	10.026	2776	2779	2780	rBV3	731	424	0.02%	0.002%
66	10.087	2793	2798	2804	rBV6	969	1386	0.06%	0.008%
67	10.222	2827	2840	2863	rBV	635557	1002176	43.06%	5.664%
68	10.457	2911	2913	2915	rBV2	445	241	0.01%	0.001%
69	10.469	2915	2917	2920	rBV4	571	426	0.02%	0.002%
70	10.624	2961	2965	2966	rVB2	688	396	0.02%	0.002%
71	10.637	2966	2969	2973	rVB3	979	703	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010521\
 Data File : VV019894.D
 Acq On : 05 Jan 2021 14:07
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.662	2973	2977	2979	rBV3	782	546	0.02%	0.003%
73	10.788	3014	3016	3017	rBV	632	187	0.01%	0.001%
74	10.881	3043	3045	3046	rBV2	604	226	0.01%	0.001%
75	10.971	3069	3073	3074	rBV2	650	413	0.02%	0.002%
76	11.010	3079	3085	3087	rBV3	821	789	0.03%	0.004%
77	11.039	3090	3094	3096	rBV3	616	319	0.01%	0.002%
78	11.071	3101	3104	3106	rBV3	1068	730	0.03%	0.004%
79	11.145	3124	3127	3128	rBV2	748	317	0.01%	0.002%
80	11.257	3150	3162	3184	rBV	1089701	1680543	72.20%	9.497%
81	11.630	3265	3278	3298	rBV	1019538	1621564	69.67%	9.164%
82	11.936	3371	3373	3375	rBV3	749	222	0.01%	0.001%
83	12.003	3391	3394	3395	rBV2	773	437	0.02%	0.002%
84	12.051	3406	3409	3411	rVB2	818	415	0.02%	0.002%
85	12.248	3468	3470	3473	rVB3	937	497	0.02%	0.003%
86	12.264	3473	3475	3477	rBV3	806	363	0.02%	0.002%
87	12.524	3553	3556	3558	rVB3	981	479	0.02%	0.003%
88	12.575	3570	3572	3574	rBV2	775	394	0.02%	0.002%
89	12.791	3637	3639	3644	rVB3	1472	981	0.04%	0.006%
90	13.235	3775	3777	3780	rBV4	930	563	0.02%	0.003%
91	13.595	3884	3889	3891	rBV3	1091	943	0.04%	0.005%
92	13.752	3934	3938	3942	rBV3	1717	1687	0.07%	0.010%




Sum of corrected areas: 17694991

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010521\
Data File : VV019894.D
Acq On : 05 Jan 2021 14:07
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

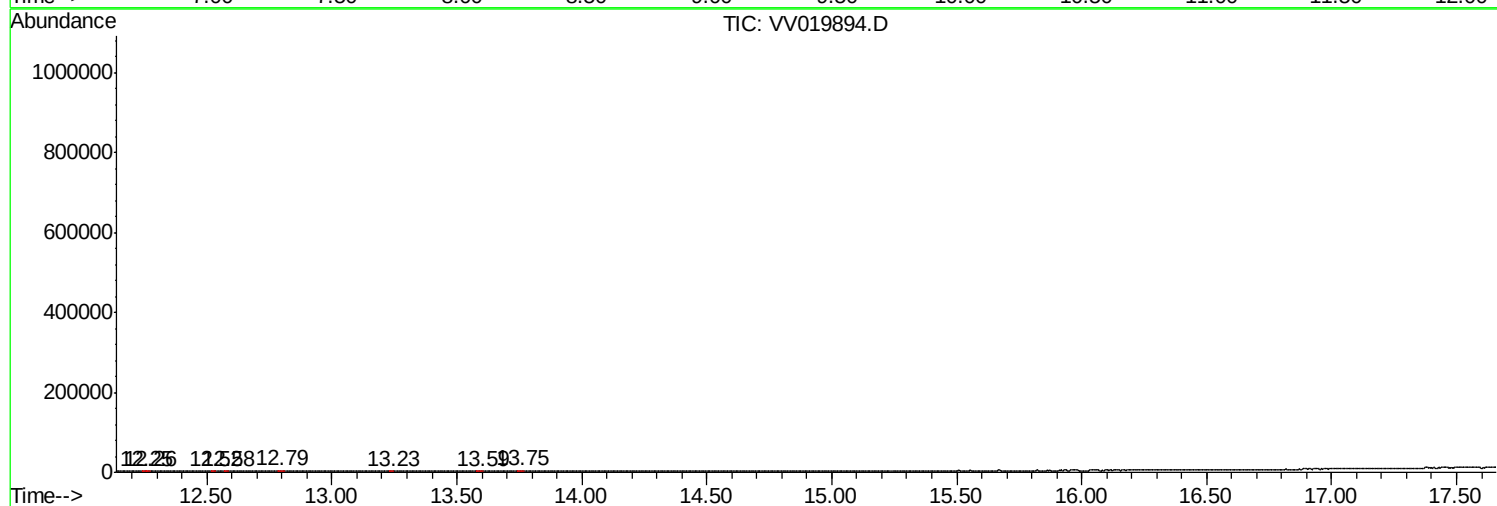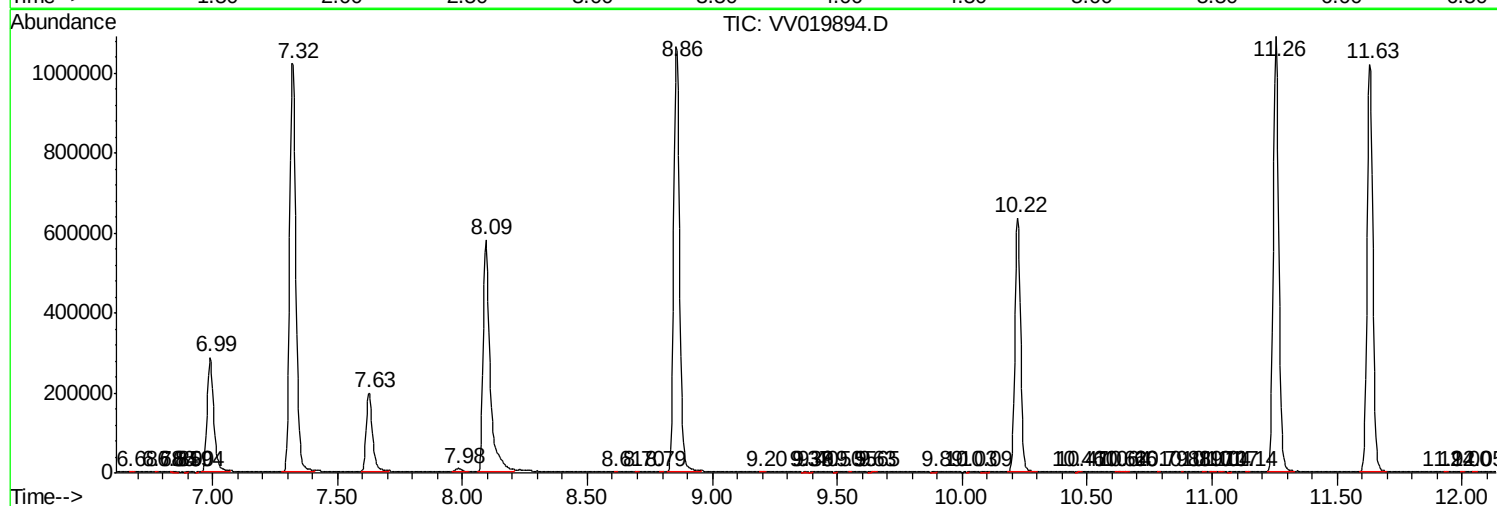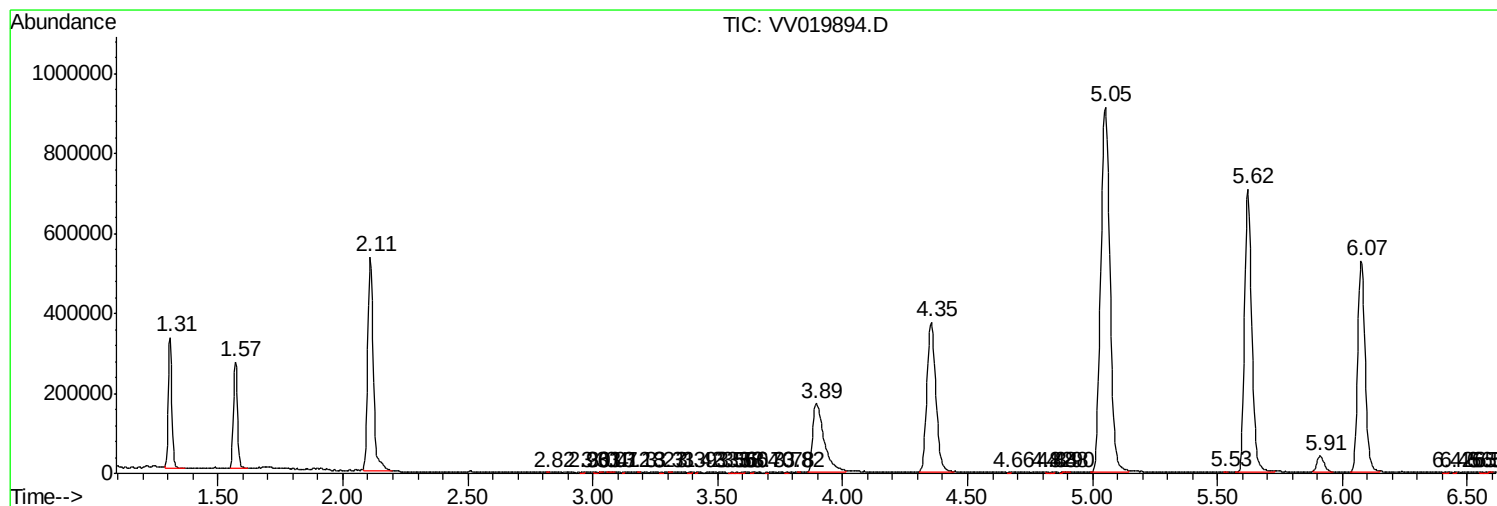

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010521\
Data File : VV019894.D
Acq On : 05 Jan 2021 14:07
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010521\
Data File : VV019894.D
Acq On : 05 Jan 2021 14:07
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc