


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV010521\
 Data File : VV019884.D
 Acq On : 05 Jan 2021 09:04
 Operator : SY/MD
 Sample : BFB75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB75

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 06 07:08:24 2021

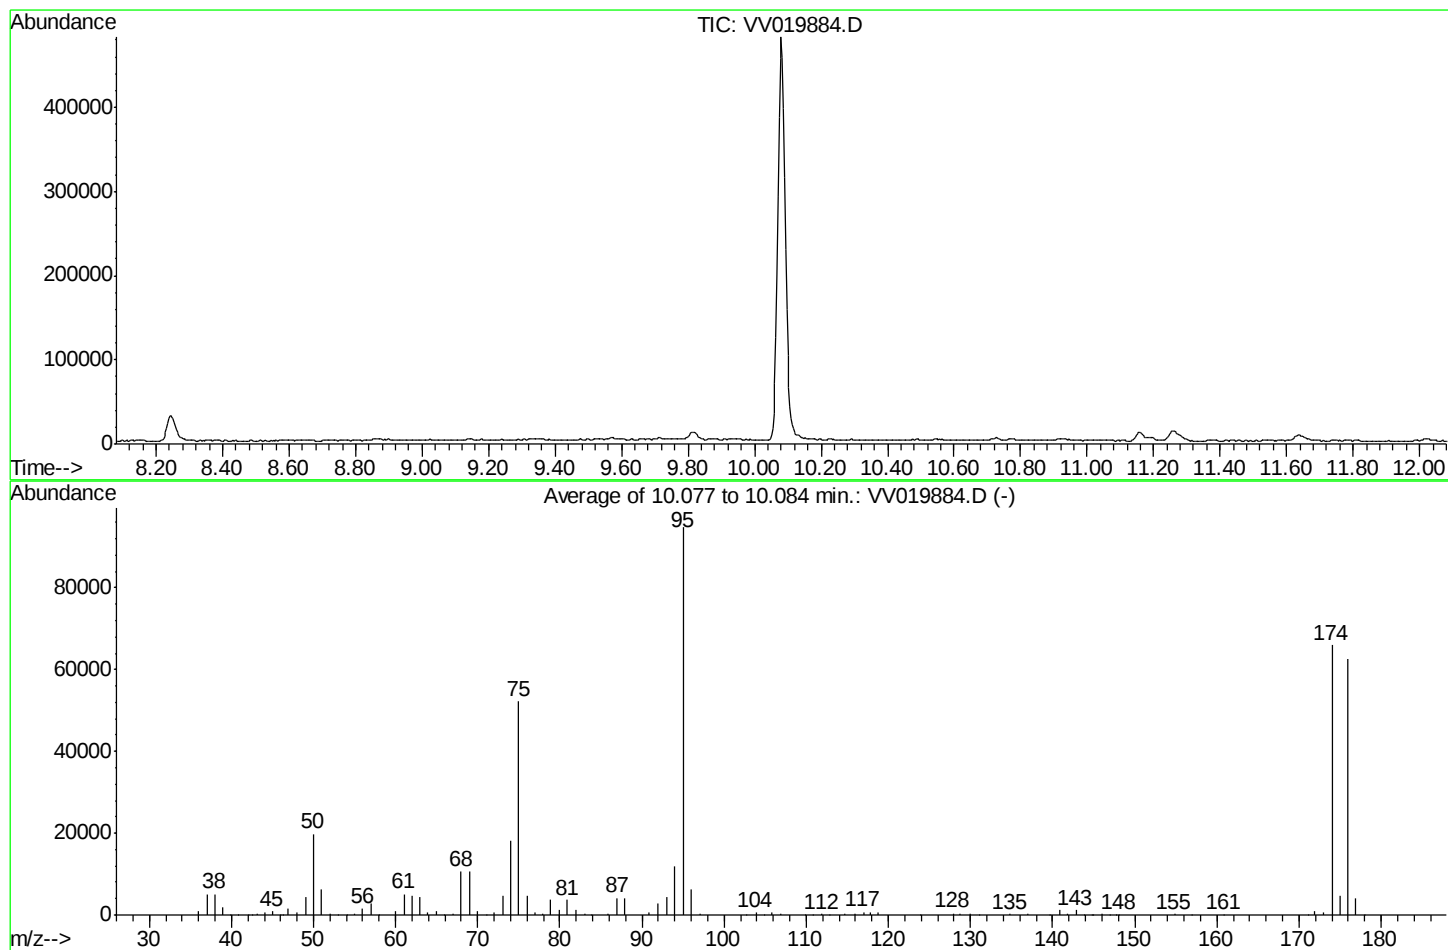

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2783

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	19864	PASS
75	95	30	80	55.1	52218	PASS
95	95	100	100	100.0	94816	PASS
96	95	5	9	6.6	6231	PASS
173	174	0.00	2	1.0	636	PASS
174	95	50	120	69.6	65952	PASS
175	174	5	9	7.0	4631	PASS
176	174	95	101	95.1	62725	PASS
177	176	5	9	6.5	4095	PASS

m/z	Abundance
36.00	3381.0
37.00	5234.0
38.00	5864.0
39.00	2027.0
40.00	418.0
40.80	125.0
42.10	189.0
43.10	201.0
44.00	1545.0
45.00	863.0
45.90	137.0
46.30	151.0
46.90	1390.0
48.00	627.0
49.00	4222.0
50.00	19968.0
51.00	6331.0
52.00	262.0
53.00	147.0
54.00	123.0
55.00	371.0
56.00	1521.0
57.00	2735.0
58.00	171.0
60.00	976.0
61.00	5020.0
62.00	4815.0
63.00	4505.0
63.90	598.0
65.00	750.0
65.90	128.0
67.00	369.0
68.00	10397.0
69.00	10574.0
70.00	996.0
71.90	726.0
73.00	4640.0
74.00	18208.0
75.00	50832.0
76.00	4881.0
77.00	716.0
77.90	484.0
78.90	3993.0
79.90	1047.0
80.90	3755.0
81.90	1080.0
83.00	139.0
83.80	119.0
85.80	234.0
87.00	4068.0
87.90	4129.0
90.90	442.0
91.90	2648.0
93.00	4342.0
94.00	11471.0
95.00	93264.0
96.00	6302.0
97.00	246.0
102.70	143.0
103.90	580.0
104.90	127.0
105.90	584.0
106.80	155.0
110.80	154.0
111.80	150.0
112.80	174.0
114.70	174.0
115.90	410.0
116.90	619.0
117.90	490.0
118.80	701.0
123.90	143.0
127.90	473.0
128.80	188.0
129.90	265.0
135.00	170.0
137.00	154.0
139.70	113.0
140.80	997.0
141.80	103.0
142.90	1077.0
143.90	118.0
144.70	222.0
145.90	224.0
147.80	101.0
148.20	109.0
154.90	219.0
156.90	129.0
171.10	154.0
171.90	885.0
173.00	894.0
174.00	62656.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

175.00	4493.0
176.00	60176.0
177.00	3959.0
177.90	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	3249.0
37.00	5372.0
38.00	6035.0
39.00	2052.0
39.90	352.0
41.00	135.0
42.10	128.0
42.50	130.0
43.10	240.0
44.00	1530.0
45.00	917.0
45.90	142.0
46.30	173.0
46.90	1523.0
47.90	690.0
49.00	4512.0
50.00	20344.0
51.00	6431.0
52.10	274.0
52.90	128.0
54.00	136.0
55.00	332.0
56.00	1591.0
57.00	2747.0
58.00	174.0
60.00	944.0
61.00	5320.0
62.00	4878.0
63.00	4639.0
63.90	514.0
65.00	908.0
65.90	128.0
67.00	444.0
68.00	10878.0
69.00	11006.0
70.00	1015.0
71.90	759.0
73.00	4824.0
74.00	18680.0
75.00	54096.0
76.00	4979.0
76.90	751.0
77.90	473.0
78.90	4029.0
79.90	1187.0
80.90	3778.0
81.90	1159.0
83.00	185.0
85.90	205.0
87.00	4300.0
87.90	4226.0
90.90	538.0
91.90	2847.0
93.00	4597.0
94.00	12224.0
95.00	98352.0
96.00	6394.0
97.00	218.0
102.70	111.0
103.90	649.0
104.90	101.0
105.90	529.0
106.90	180.0
109.90	110.0
110.80	133.0
111.90	175.0
112.80	172.0
114.70	186.0
115.90	426.0
117.00	757.0
117.90	522.0
118.80	709.0
127.90	477.0
128.80	230.0
129.90	317.0
131.00	125.0
134.80	215.0
136.90	207.0
140.90	1181.0
141.80	148.0
142.90	1258.0
143.90	131.0
144.70	185.0
145.90	192.0
146.90	107.0
147.80	133.0
154.80	203.0
156.80	117.0
160.90	117.0
171.10	154.0
171.90	922.0
173.00	1016.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

174.00	68584.0
175.00	4819.0
176.00	64872.0
177.00	4196.0
178.00	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	2944.0
37.00	5083.0
38.00	5684.0
39.00	1895.0
39.90	332.0
41.10	161.0
42.00	107.0
42.60	168.0
43.10	245.0
44.00	1374.0
45.00	877.0
46.00	147.0
46.30	167.0
47.00	1564.0
47.90	697.0
49.00	4448.0
50.00	19280.0
51.00	6060.0
52.10	293.0
52.90	117.0
55.00	259.0
56.00	1477.0
57.00	2633.0
58.00	144.0
60.00	893.0
61.00	5161.0
62.00	4589.0
63.00	4266.0
63.90	379.0
65.00	993.0
67.00	459.0
68.00	10436.0
69.00	10066.0
70.00	922.0
71.10	118.0
71.90	695.0
73.00	4543.0
74.00	17448.0
75.00	51728.0
76.00	4327.0
76.90	709.0
77.90	425.0
78.90	3593.0
79.90	1254.0
80.90	3545.0
81.90	1089.0
83.00	214.0
85.90	177.0
87.00	4004.0
87.90	3992.0
90.90	587.0
91.90	2662.0
93.00	4379.0
94.00	11607.0
95.00	92832.0
96.00	5998.0
97.00	202.0
103.90	565.0
104.90	114.0
105.80	413.0
106.90	198.0
109.90	121.0
110.90	123.0
112.00	195.0
112.90	129.0
114.70	177.0
115.90	413.0
117.00	779.0
117.80	501.0
118.80	614.0
127.90	431.0
128.70	232.0
129.90	338.0
131.00	138.0
134.80	207.0
136.80	226.0
140.90	1233.0
141.80	256.0
142.90	1231.0
144.90	142.0
146.00	142.0
147.00	104.0
148.00	177.0
154.90	178.0
156.80	107.0
160.90	143.0
171.10	138.0
172.00	931.0
174.00	66616.0
175.00	4582.0
175.90	63128.0
176.90	4131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

178.00

120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	2110.0
37.10	224.0
37.90	795.0
38.80	119.0
39.20	110.0
39.80	276.0
41.10	147.0
41.80	121.0
42.00	125.0
44.00	770.0
53.00	125.0
76.80	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75