

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW010522\
 Data File : VW024279.D
 Acq On : 05 Jan 2022 15:33
 Operator : SY/MD
 Sample : N1025-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH3

Quant Time: Jan 06 01:00:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 06 00:59:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	231939	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	219482	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	107393	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	78331	46.926	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.860%
7) Chloroethane-d5	1.568	69	62223	49.070	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.140%
11) 1,1-Dichloroethene-d2	2.108	63	115873	37.142	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.280%
21) 2-Butanone-d5	3.889	46	84523	90.885	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.880%
24) Chloroform-d	4.349	84	144569	47.387	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.780%
26) 1,2-Dichloroethane-d4	5.030	65	98349	48.149	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.300%
32) Benzene-d6	5.050	84	282754	49.368	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.740%
36) 1,2-Dichloropropane-d6	6.069	67	79085	49.269	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.540%
41) Toluene-d8	7.313	98	267295	48.200	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.400%
43) trans-1,3-Dichloroprop...	7.622	79	42407	45.880	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.760%
47) 2-Hexanone-d5	8.088	63	58943	84.521	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.520%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	97265	42.401	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	112192	52.411	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.820%
Target Compounds						
					Qvalue	
13) Acetone	2.182	43	3674	4.001	ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010522\
Data File : VV024279.D
Acq On : 05 Jan 2022 15:33
Operator : SY/MD
Sample : N1025-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLH3

Quant Time: Jan 06 01:00:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 06 00:59:13 2022
Response via : Initial Calibration

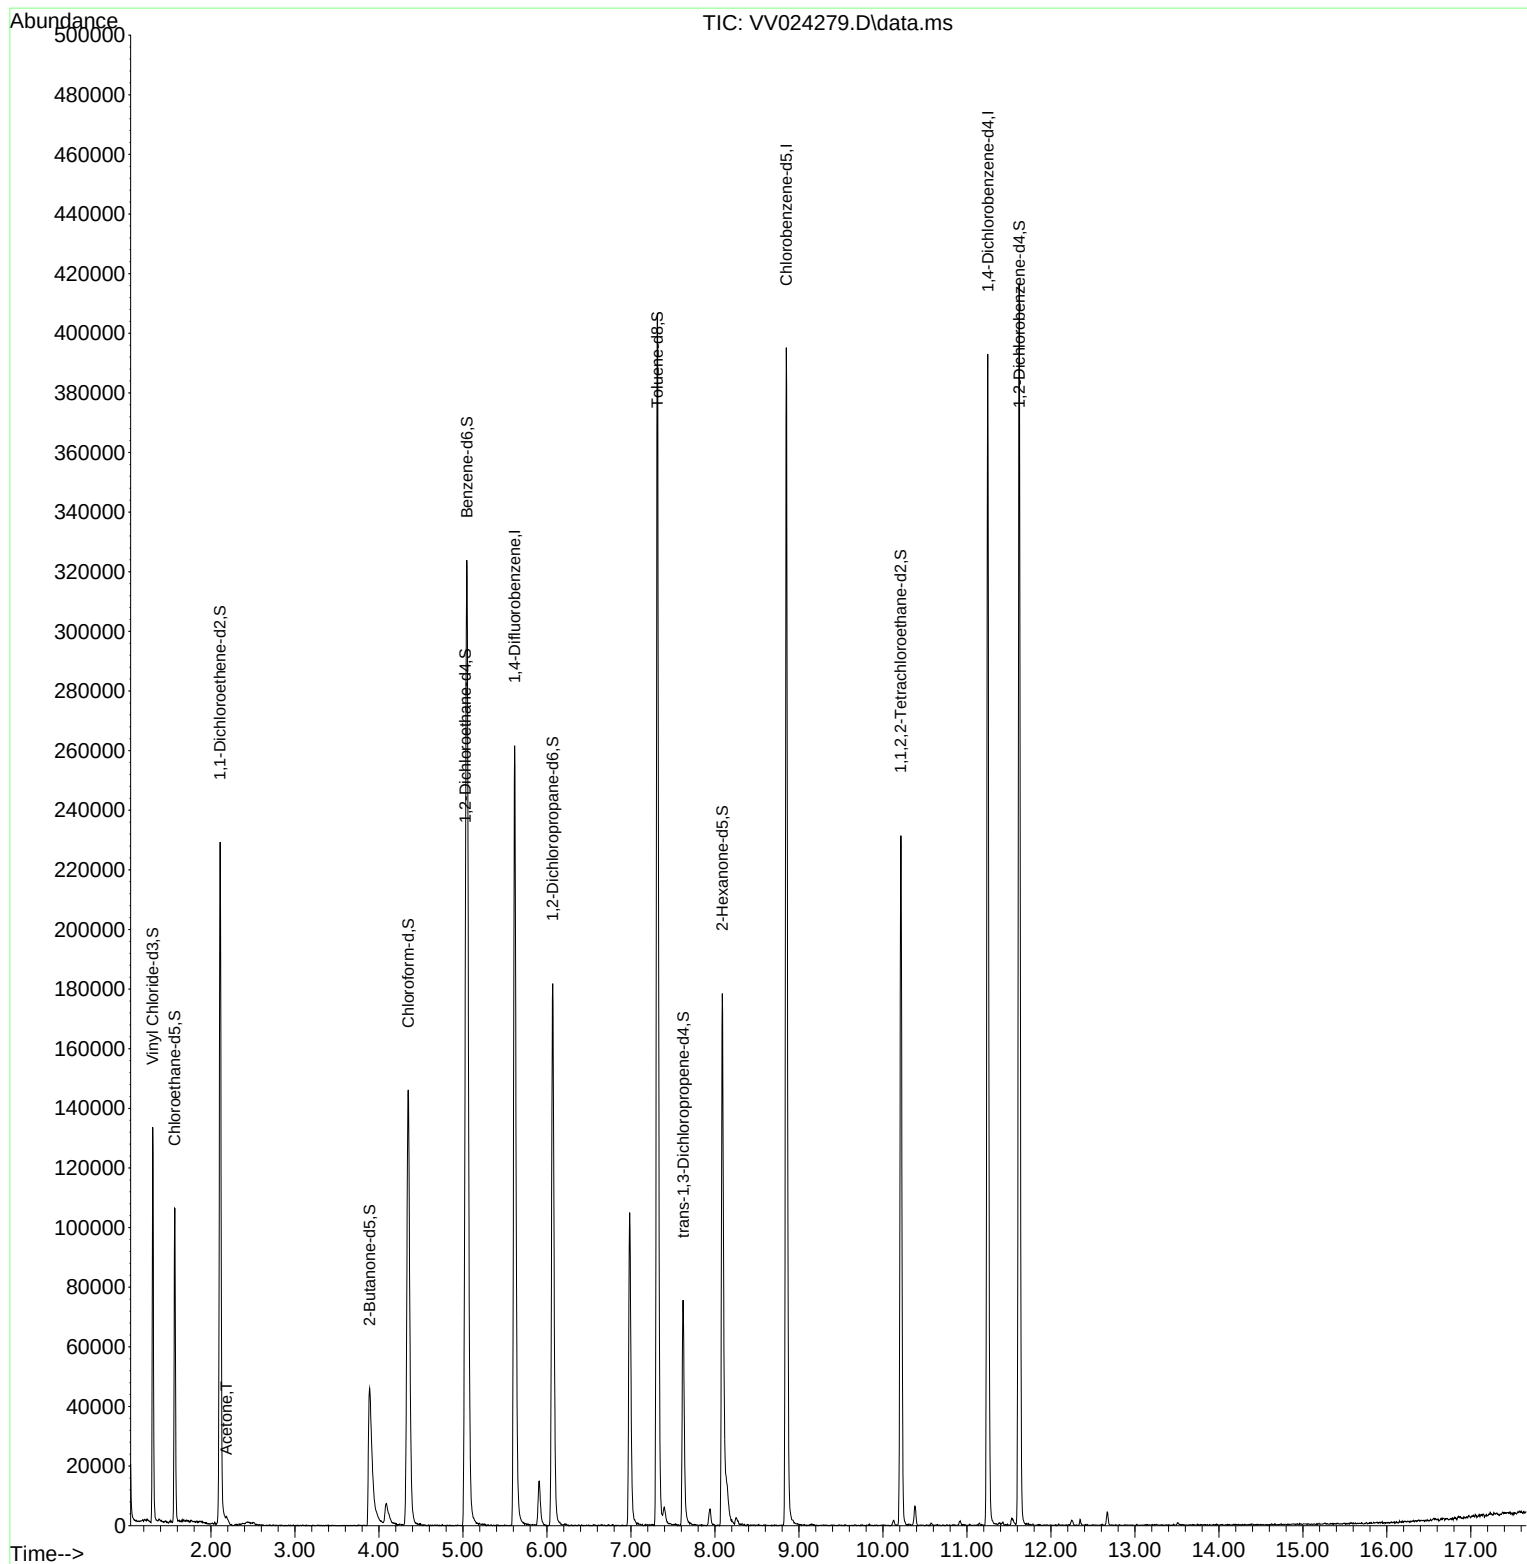

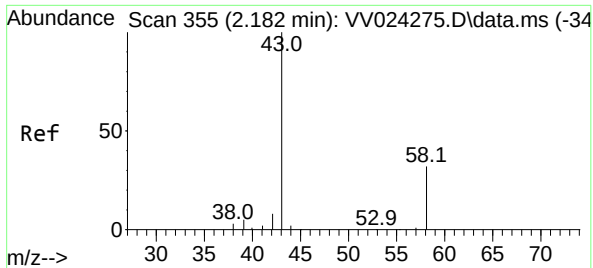

#13
 Acetone
 Concen: 4.001 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV024279.D
 Acq: 05 Jan 2022 15:33

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH3

Tgt Ion: 43 Resp: 3674
 Ion Ratio Lower Upper
 43 100
 58 19.7 0.0 63.0

