

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW010522\
 Data File : VW024283.D
 Acq On : 05 Jan 2022 17:20
 Operator : SY/MD
 Sample : N1009-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLG4

Quant Time: Jan 06 01:01:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 06 00:59:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	248096	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	232979	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	118991	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	83916	46.998	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.000%
7) Chloroethane-d5	1.571	69	65311	48.151	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.300%
11) 1,1-Dichloroethene-d2	2.111	63	124372	37.270	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.540%
21) 2-Butanone-d5	3.883	46	91181	91.659	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.660%
24) Chloroform-d	4.349	84	154649	47.390	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.780%
26) 1,2-Dichloroethane-d4	5.030	65	105309	48.199	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.400%
32) Benzene-d6	5.050	84	298139	49.038	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.080%
36) 1,2-Dichloropropane-d6	6.069	67	84952	49.858	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.720%
41) Toluene-d8	7.316	98	284182	48.277	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.560%
43) trans-1,3-Dichloroprop...	7.622	79	45180	46.048	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.100%
47) 2-Hexanone-d5	8.088	63	66523	89.864	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.860%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	108002	44.354	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.700%
66) 1,2-Dichlorobenzene-d4	11.625	152	121562	51.253	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.500%
Target Compounds						
					Qvalue	
13) Acetone	2.182	43	4375	4.454	ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010522\
Data File : VV024283.D
Acq On : 05 Jan 2022 17:20
Operator : SY/MD
Sample : N1009-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLG4

Quant Time: Jan 06 01:01:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 06 00:59:13 2022
Response via : Initial Calibration

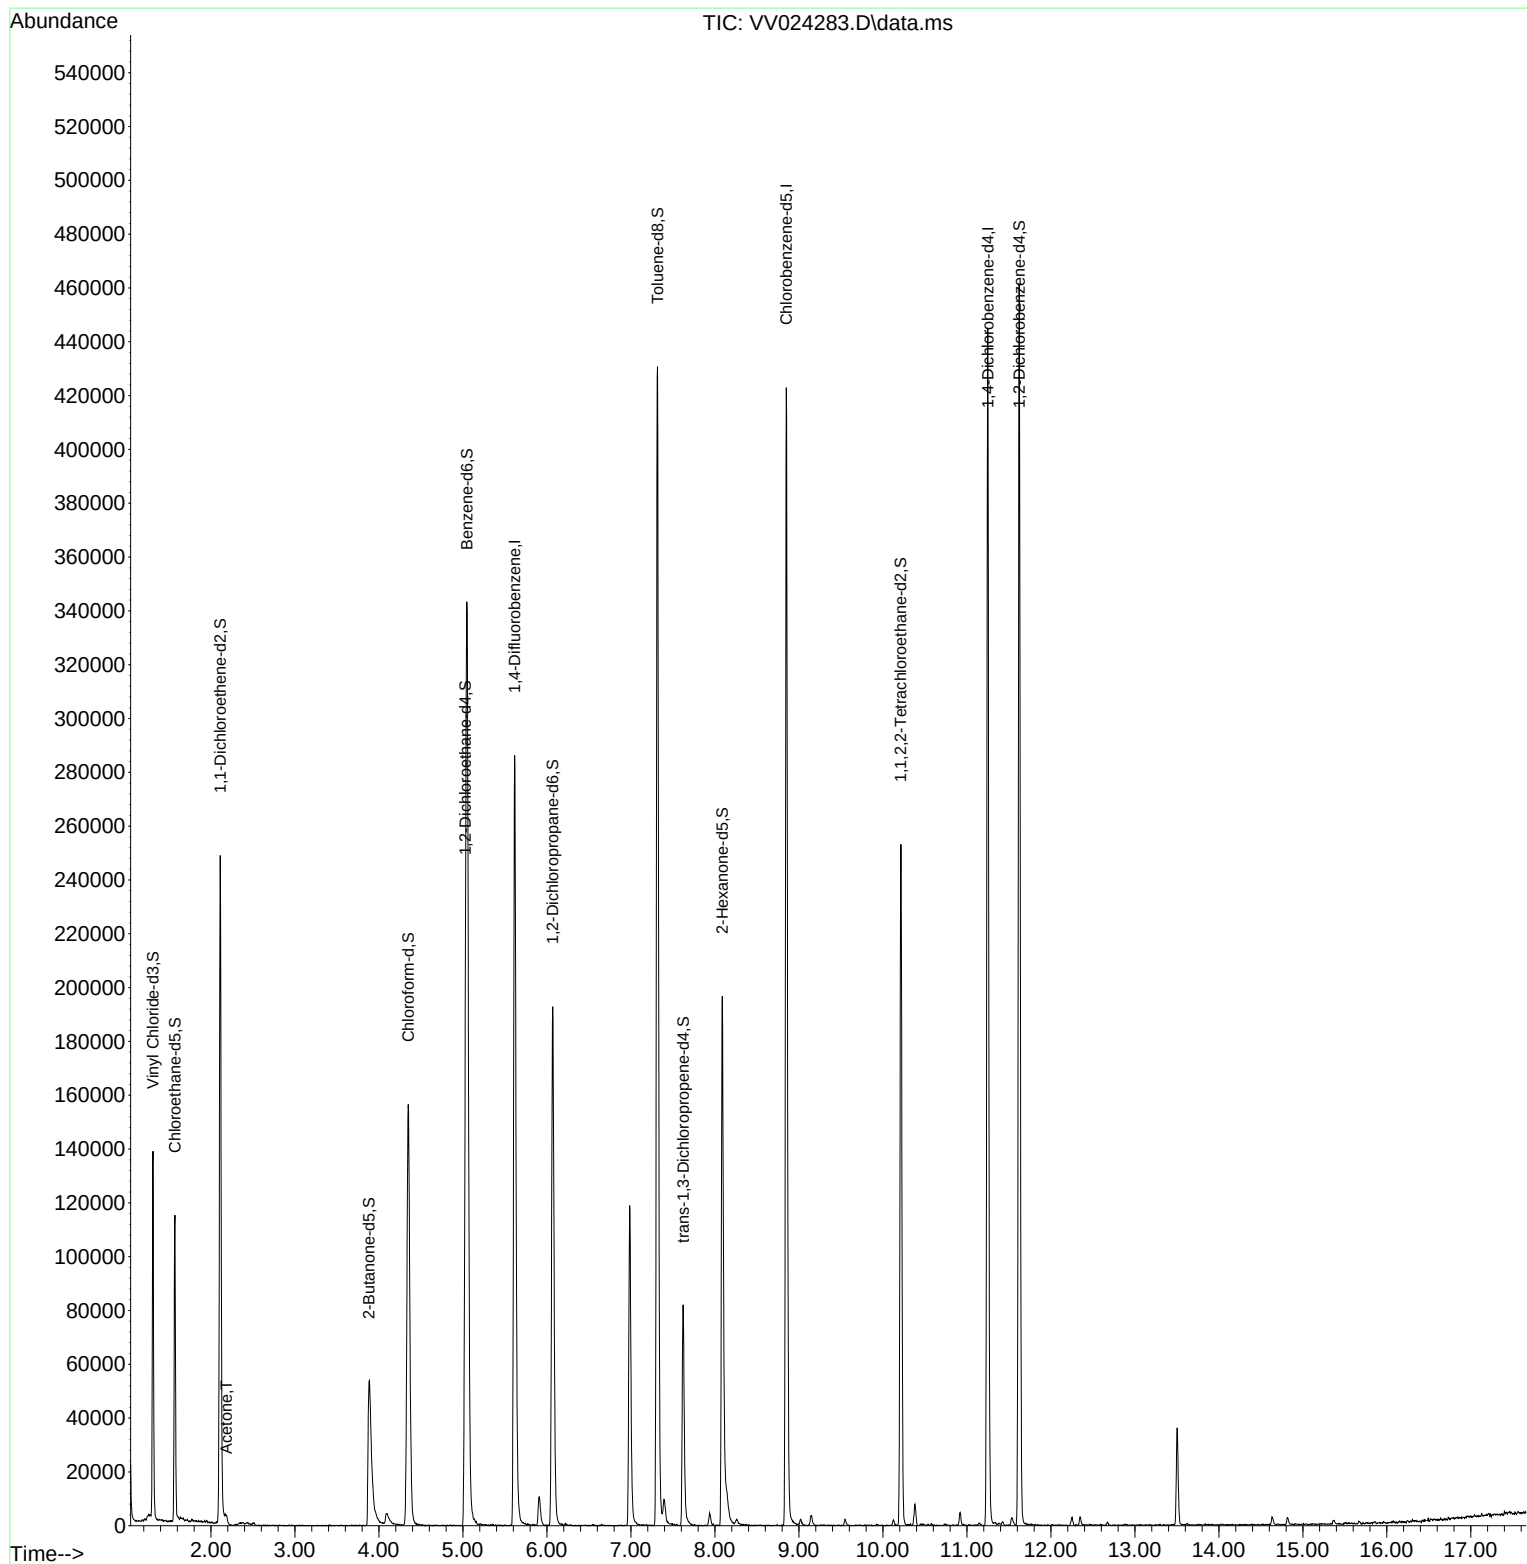

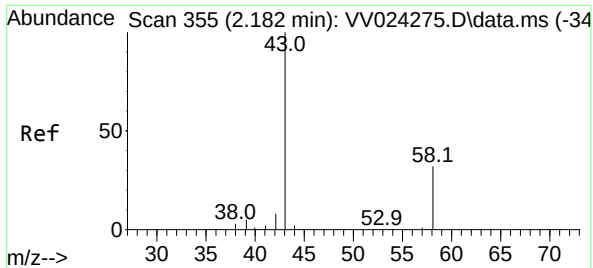

#13
 Acetone
 Concen: 4.454 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV024283.D
 Acq: 05 Jan 2022 17:20

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLG4

Tgt Ion: 43 Resp: 4375
 Ion Ratio Lower Upper
 43 100
 58 18.7 0.0 63.0

