

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010522\
 Data File : VV024278.D
 Acq On : 05 Jan 2022 15:10
 Operator : SY/MD
 Sample : N1025-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

Signal : TIC: VV024278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	139217	138345	16.20%	2.170%
2	1.568	157	164	176	rBV	109863	121161	14.19%	1.900%
3	2.654	500	502	504	rBB	256	115	0.01%	0.002%
4	2.667	504	506	508	rBV	128	87	0.01%	0.001%
5	2.715	518	521	525	rBV	156	174	0.02%	0.003%
6	2.757	531	534	535	rBV	134	95	0.01%	0.001%
7	2.793	543	545	549	rBV	130	139	0.02%	0.002%
8	2.899	575	578	581	rBV	245	209	0.02%	0.003%
9	2.966	595	599	601	rBB	222	147	0.02%	0.002%
10	3.040	619	622	624	rBB	271	126	0.01%	0.002%
11	3.169	658	662	666	rBB	166	196	0.02%	0.003%
12	3.449	746	749	751	rBV	226	110	0.01%	0.002%
13	3.516	768	770	772	rBV	139	91	0.01%	0.001%
14	3.677	817	820	823	rBB	260	167	0.02%	0.003%
15	3.712	829	831	834	rBB	224	146	0.02%	0.002%
16	3.744	835	841	844	rBB	170	189	0.02%	0.003%
17	3.883	874	884	920	rBV	44428	138555	16.22%	2.173%
18	4.346	1012	1028	1057	rBV	147360	363217	42.53%	5.697%
19	4.606	1107	1109	1113	rBB	155	125	0.01%	0.002%
20	4.667	1123	1128	1129	rBV	210	185	0.02%	0.003%
21	4.686	1132	1134	1136	rVB	249	94	0.01%	0.001%
22	4.735	1146	1149	1155	rBV	143	209	0.02%	0.003%
23	4.844	1180	1183	1185	rBV	264	170	0.02%	0.003%
24	4.915	1202	1205	1208	rBB2	280	192	0.02%	0.003%
25	5.043	1228	1245	1272	rBV2	327651	854032	100.00%	13.396%
26	5.339	1336	1337	1338	rBV2	312	110	0.01%	0.002%
27	5.442	1366	1369	1371	rBB	121	87	0.01%	0.001%
28	5.458	1371	1374	1376	rBB	150	98	0.01%	0.002%
29	5.487	1381	1383	1386	rBB2	266	167	0.02%	0.003%
30	5.567	1405	1408	1410	rBV	263	183	0.02%	0.003%
31	5.612	1410	1422	1446	rBV	283301	567083	66.40%	8.895%
32	5.825	1484	1488	1491	rBV2	331	328	0.04%	0.005%
33	5.902	1502	1512	1528	rBV3	12363	26950	3.16%	0.423%
34	6.002	1541	1543	1546	rBB	258	120	0.01%	0.002%
35	6.066	1550	1563	1588	rBV	184584	376368	44.07%	5.904%
36	6.214	1605	1609	1611	rBV2	962	559	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010522\
 Data File : VV024278.D
 Acq On : 05 Jan 2022 15:10
 Operator : SY/MD
 Sample : N1025-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	6.249	1615	1620	1623	rVB3	408	365	0.04%	0.006%
38	6.268	1624	1626	1629	rBV3	218	128	0.01%	0.002%
39	6.304	1635	1637	1639	rBB3	258	98	0.01%	0.002%
40	6.558	1712	1716	1717	rBV3	222	111	0.01%	0.002%
41	6.622	1734	1736	1739	rBB	284	170	0.02%	0.003%
42	6.645	1739	1743	1746	rBV2	370	307	0.04%	0.005%
43	6.690	1755	1757	1760	rBB	159	108	0.01%	0.002%
44	6.825	1795	1799	1801	rBB	139	113	0.01%	0.002%
45	6.889	1817	1819	1820	rBV	223	90	0.01%	0.001%
46	6.911	1824	1826	1829	rBB	134	92	0.01%	0.001%
47	6.982	1837	1848	1873	rBV2	107611	196274	22.98%	3.079%
48	7.169	1905	1906	1908	rBV	451	183	0.02%	0.003%
49	7.230	1922	1925	1927	rBV	132	111	0.01%	0.002%
50	7.313	1937	1951	1970	rBV	413583	717324	83.99%	11.252%
51	7.583	2033	2035	2036	rBV	272	151	0.02%	0.002%
52	7.619	2036	2046	2071	rVV2	77294	134765	15.78%	2.114%
53	7.786	2093	2098	2102	rBV4	345	392	0.05%	0.006%
54	7.854	2113	2119	2120	rBV2	367	383	0.04%	0.006%
55	7.982	2156	2159	2163	rBV2	580	519	0.06%	0.008%
56	8.021	2167	2171	2173	rBV2	232	148	0.02%	0.002%
57	8.085	2181	2191	2233	rBV	168793	328362	38.45%	5.151%
58	8.358	2271	2276	2278	rBV2	393	362	0.04%	0.006%
59	8.619	2355	2357	2359	rBV	137	95	0.01%	0.001%
60	8.648	2364	2366	2368	rBV2	247	137	0.02%	0.002%
61	8.738	2390	2394	2396	rBV	399	289	0.03%	0.005%
62	8.850	2417	2429	2452	rBV	426516	687239	80.47%	10.780%
63	9.079	2496	2500	2503	rBV2	278	247	0.03%	0.004%
64	9.143	2514	2520	2522	rBV	673	595	0.07%	0.009%
65	9.201	2533	2538	2540	rBV	223	234	0.03%	0.004%
66	9.304	2567	2570	2575	rBB2	290	290	0.03%	0.005%
67	9.333	2575	2579	2581	rBV	220	187	0.02%	0.003%
68	9.471	2619	2622	2623	rBV	224	118	0.01%	0.002%
69	9.532	2638	2641	2643	rBB	156	110	0.01%	0.002%
70	9.545	2643	2645	2646	rBV	209	90	0.01%	0.001%
71	9.567	2651	2652	2656	rBV	234	144	0.02%	0.002%
72	9.651	2676	2678	2681	rBV	158	127	0.01%	0.002%
73	9.718	2695	2699	2702	rBB	255	166	0.02%	0.003%
74	9.741	2702	2706	2709	rBV	180	212	0.02%	0.003%
75	9.799	2721	2724	2727	rBV	148	150	0.02%	0.002%
76	9.844	2736	2738	2739	rBV	265	126	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010522\
 Data File : VV024278.D
 Acq On : 05 Jan 2022 15:10
 Operator : SY/MD
 Sample : N1025-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

77	9.931	2763	2765	2767	rBV	268	139	0.02%	0.002%
78	9.966	2773	2776	2779	rBV	135	141	0.02%	0.002%
79	10.008	2785	2789	2790	rBV	248	141	0.02%	0.002%
80	10.062	2803	2806	2810	rBB	170	156	0.02%	0.002%
81	10.091	2812	2815	2818	rBV	382	270	0.03%	0.004%
82	10.214	2842	2853	2871	rBV	230698	359472	42.09%	5.639%
83	10.435	2918	2922	2925	rBV	187	177	0.02%	0.003%
84	10.480	2933	2936	2938	rBV	127	88	0.01%	0.001%
85	10.551	2956	2958	2961	rBV	398	292	0.03%	0.005%
86	10.632	2981	2983	2989	rBV2	412	371	0.04%	0.006%
87	10.673	2993	2996	2998	rBV	185	150	0.02%	0.002%
88	11.075	3118	3121	3123	rBV	178	158	0.02%	0.002%
89	11.246	3164	3174	3194	rBV	437449	666783	78.07%	10.459%
90	11.471	3240	3244	3248	rBB	205	213	0.02%	0.003%
91	11.496	3248	3252	3256	rBV	171	235	0.03%	0.004%
92	11.538	3259	3265	3276	rVV5	1855	3510	0.41%	0.055%
93	11.622	3280	3291	3316	rVB	430893	673836	78.90%	10.570%
94	11.786	3340	3342	3346	rVB3	987	518	0.06%	0.008%
95	11.905	3378	3379	3382	rVB2	256	94	0.01%	0.001%
96	11.979	3400	3402	3406	rBV	227	103	0.01%	0.002%
97	12.201	3467	3471	3474	rBV	279	271	0.03%	0.004%
98	12.673	3611	3618	3625	rBV5	4502	6247	0.73%	0.098%
99	13.348	3826	3828	3833	rVB2	272	148	0.02%	0.002%
100	14.030	4037	4040	4046	rBV	290	319	0.04%	0.005%




Sum of corrected areas: 6375273

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010522\
Data File : VV024278.D
Acq On : 05 Jan 2022 15:10
Operator : SY/MD
Sample : N1025-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

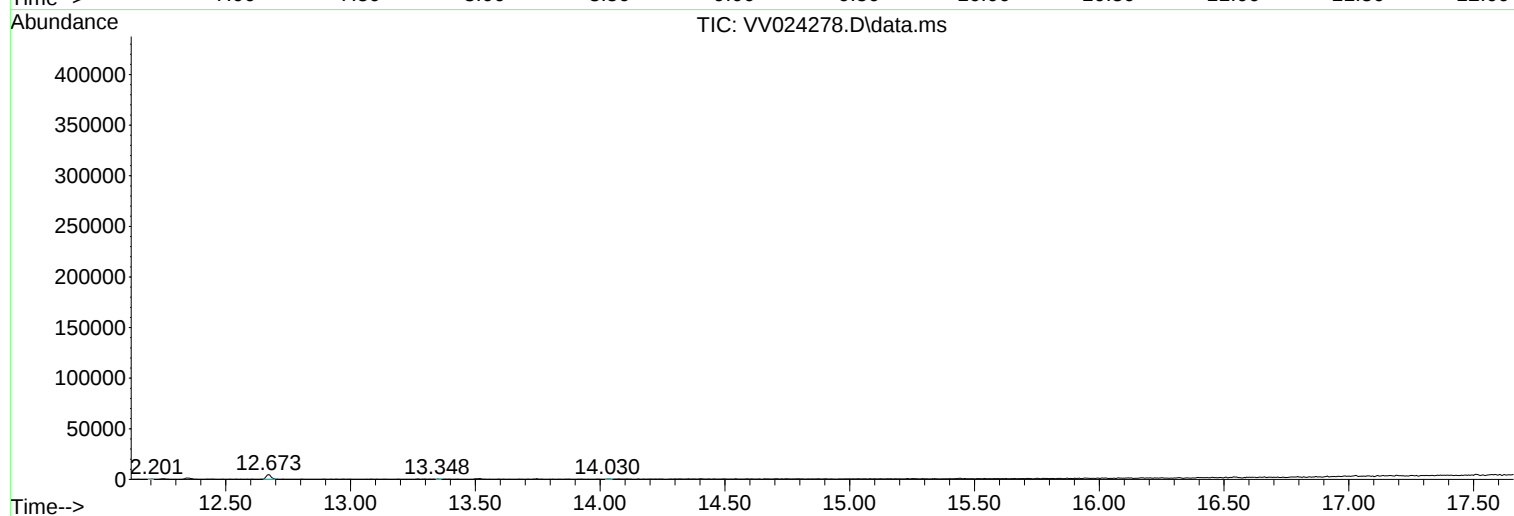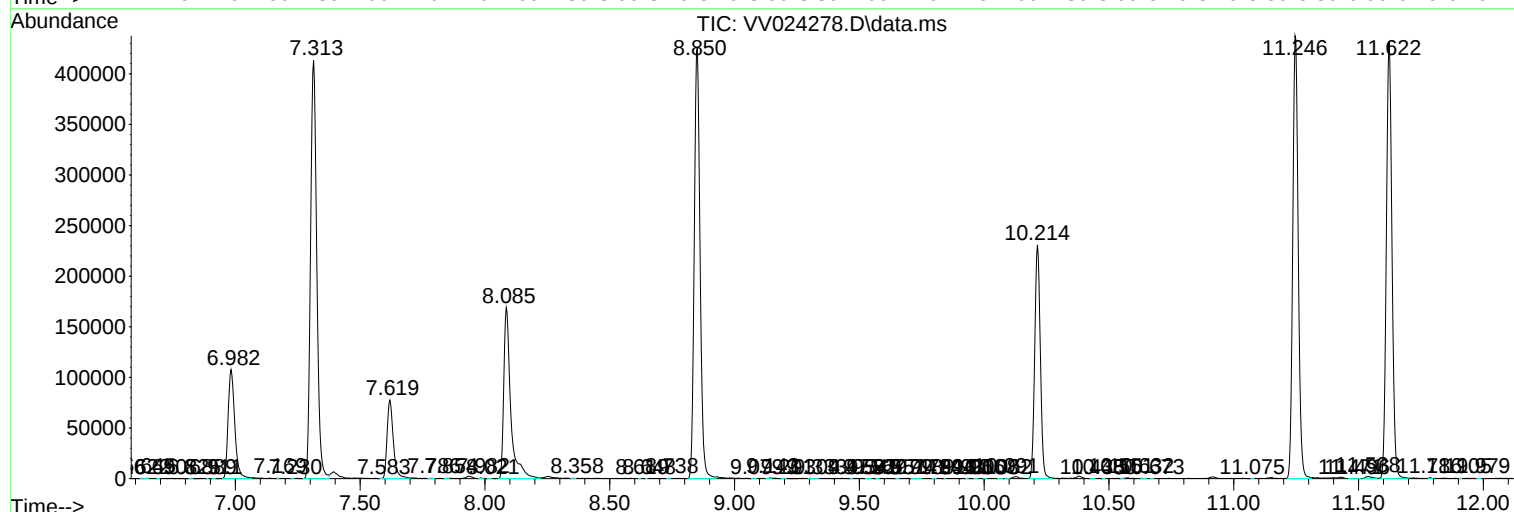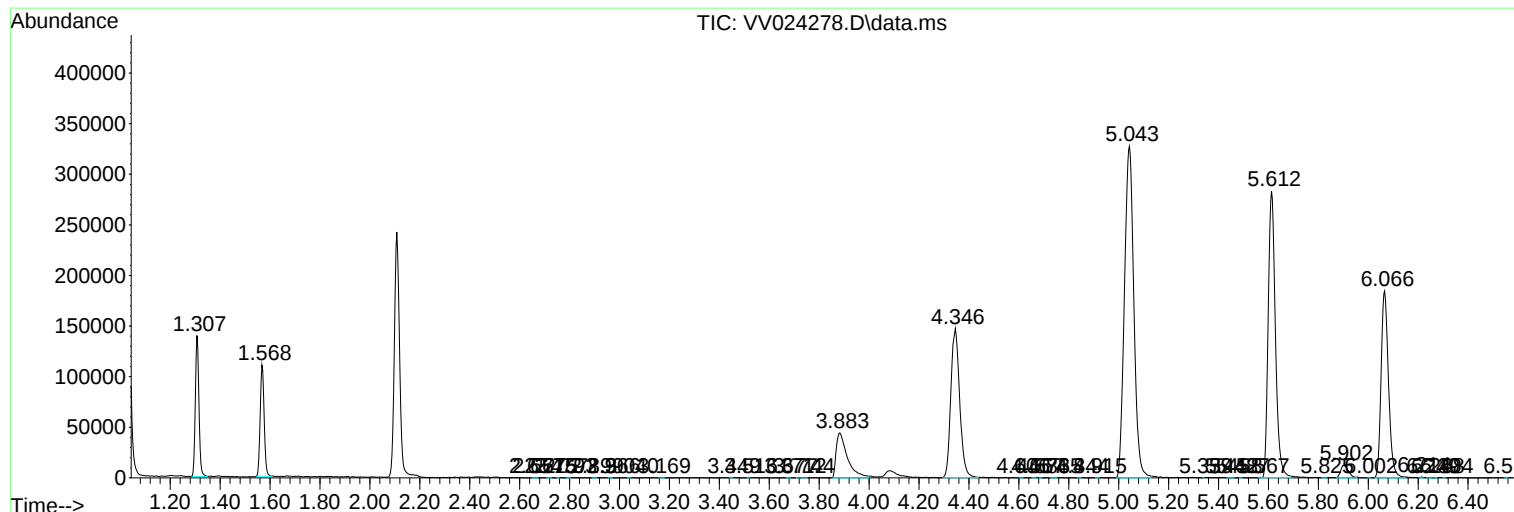

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010522\
Data File : VV024278.D
Acq On : 05 Jan 2022 15:10
Operator : SY/MD
Sample : N1025-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010522\
Data File : VV024278.D
Acq On : 05 Jan 2022 15:10
Operator : SY/MD
Sample : N1025-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------