
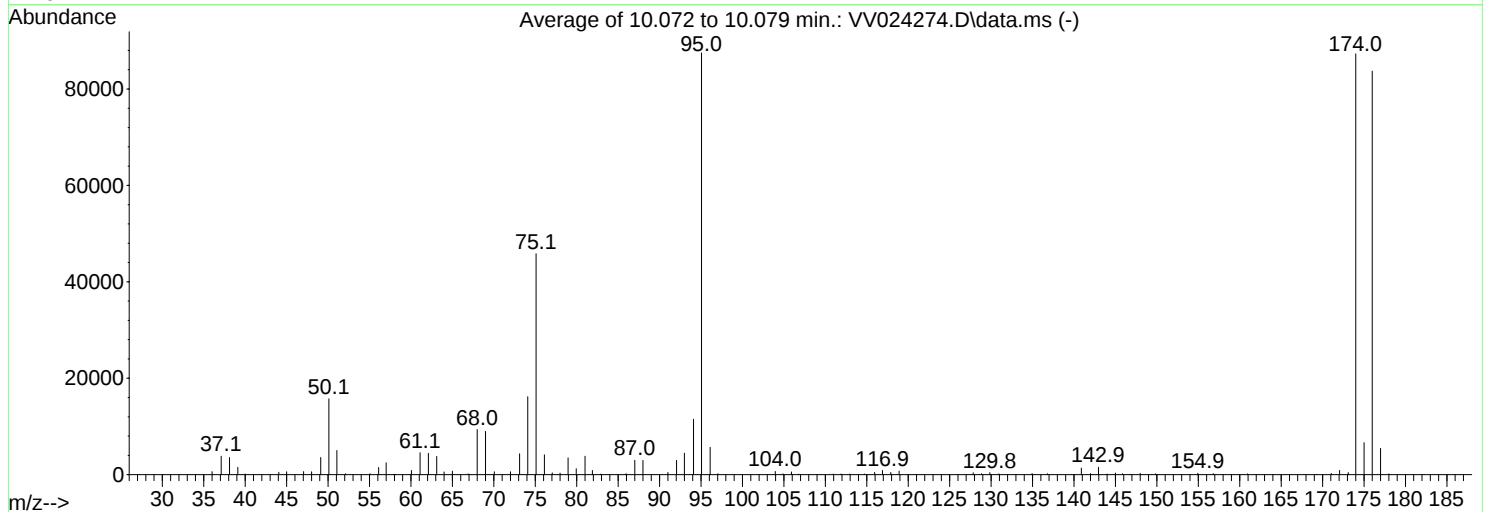


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010522\
Data File : VV024274.D
Acq On : 05 Jan 2022 10:20
Operator : SY/MD
Sample : BFB251
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB251

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Title : VOC Analysis
Last Update : Fri Jan 07 01:34:41 2022

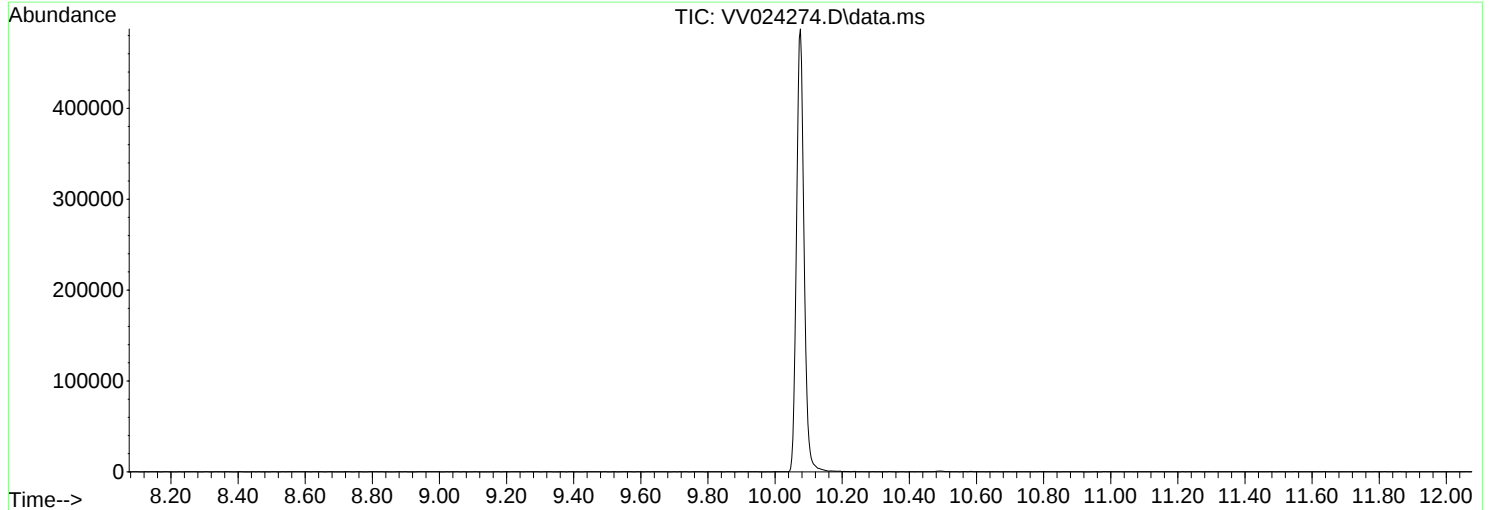

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	15739	PASS
75	95	30	80	52.4	45853	PASS
95	95	100	100	100.0	87501	PASS
96	95	5	9	6.5	5667	PASS
173	174	0.00	2	0.5	436	PASS
174	95	50	120	99.8	87312	PASS
175	174	5	9	7.6	6648	PASS
176	174	95	105	95.9	83699	PASS
177	176	5	10	6.5	5447	PASS

m/z	Abundance
44.10	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB251

m/z	Abundance
36.00	634.0
37.10	3934.0
38.10	3496.0
39.10	1611.0
40.00	192.0
44.10	624.0
45.00	632.0
47.00	573.0
48.00	578.0
49.10	3737.0
50.10	16327.0
51.10	5304.0
52.10	233.0
55.10	212.0
56.10	1470.0
57.00	2605.0
57.90	122.0
60.00	862.0
61.10	4677.0
62.10	4544.0
63.10	4197.0
64.00	587.0
65.00	799.0
66.90	266.0
68.00	9374.0
69.00	9279.0
70.10	673.0
72.00	615.0
73.10	4445.0
74.10	16496.0
75.10	46496.0
76.10	4270.0
77.10	373.0
78.00	330.0
79.00	3559.0
79.90	1235.0
81.00	3796.0
81.90	813.0
83.00	105.0
86.00	235.0
87.00	3031.0
88.00	3119.0
91.00	498.0
92.10	3017.0
93.00	4415.0
94.10	11810.0
95.00	89800.0
96.10	6044.0
97.10	183.0
104.00	695.0
104.90	152.0
105.90	504.0
106.80	146.0
110.90	148.0
111.80	154.0
112.90	123.0
114.80	127.0
115.90	429.0
116.90	855.0
117.90	444.0
118.90	702.0
127.80	376.0
128.90	227.0
129.90	454.0
130.90	149.0
134.90	206.0
136.80	199.0
140.90	1361.0
142.00	186.0
142.90	1479.0
144.00	116.0
145.00	347.0
145.90	228.0
146.80	107.0
148.00	243.0
149.80	117.0
154.90	328.0
156.80	226.0
161.00	172.0
169.30	102.0
171.00	254.0
172.00	857.0
173.10	1309.0
174.00	86112.0
175.00	6517.0
176.00	82320.0
177.00	5545.0
178.00	214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB251

m/z	Abundance
36.00	674.0
37.10	3912.0
38.10	3701.0
39.10	1606.0
40.00	141.0
44.10	669.0
45.00	599.0
47.10	661.0
48.00	606.0
49.10	3604.0
50.10	16294.0
51.00	5213.0
52.10	219.0
55.00	189.0
56.10	1558.0
57.00	2540.0
60.00	890.0
61.10	4721.0
62.10	4517.0
63.10	3900.0
64.00	569.0
65.00	770.0
66.90	257.0
68.00	9863.0
69.00	9298.0
70.00	593.0
72.00	665.0
73.10	4440.0
74.10	16712.0
75.10	47496.0
76.10	4312.0
77.10	390.0
78.00	361.0
78.90	3604.0
79.90	1258.0
81.00	3977.0
81.90	901.0
82.90	113.0
86.00	226.0
87.00	3092.0
88.00	3102.0
91.00	497.0
92.00	3052.0
93.00	4605.0
94.10	11857.0
95.10	90344.0
96.10	5784.0
97.00	206.0
103.90	711.0
104.90	188.0
105.90	576.0
106.80	135.0
111.00	167.0
111.90	138.0
113.00	120.0
114.70	161.0
116.00	511.0
116.90	879.0
117.90	482.0
118.90	766.0
127.90	412.0
128.90	207.0
129.90	429.0
131.00	165.0
135.00	221.0
136.80	199.0
140.90	1424.0
142.00	202.0
142.90	1564.0
144.00	130.0
145.00	335.0
145.80	212.0
146.80	116.0
148.00	267.0
149.00	108.0
149.90	187.0
154.90	279.0
156.80	238.0
158.90	111.0
161.00	203.0
169.30	114.0
171.00	265.0
172.10	911.0
174.00	90384.0
175.00	6850.0
176.00	86624.0
177.00	5546.0
178.00	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB251

m/z	Abundance
36.00	640.0
37.10	3601.0
38.10	3512.0
39.10	1400.0
40.00	114.0
44.00	632.0
45.00	603.0
45.90	104.0
47.10	704.0
48.00	577.0
49.10	3288.0
50.10	14595.0
51.10	4549.0
52.10	206.0
55.00	176.0
56.10	1467.0
57.00	2272.0
58.10	107.0
60.10	856.0
61.10	4245.0
62.10	4166.0
63.10	3294.0
64.00	505.0
65.00	652.0
67.10	233.0
68.00	8837.0
69.00	8308.0
70.00	507.0
72.00	561.0
73.10	4113.0
74.10	15341.0
75.10	43568.0
76.10	3821.0
77.00	368.0
78.00	312.0
78.90	3253.0
80.00	1182.0
81.00	3718.0
81.90	887.0
82.80	125.0
85.90	165.0
87.00	2867.0
88.00	2673.0
91.00	436.0
92.00	2756.0
93.00	4350.0
94.10	10817.0
95.10	82360.0
96.10	5172.0
97.00	182.0
103.90	586.0
104.90	182.0
105.90	589.0
111.00	138.0
112.00	110.0
113.00	127.0
114.70	134.0
116.00	492.0
116.90	819.0
117.90	505.0
118.90	682.0
127.90	402.0
128.80	178.0
129.80	376.0
130.90	178.0
135.00	234.0
136.80	222.0
140.90	1285.0
142.00	180.0
143.00	1545.0
144.00	135.0
145.00	352.0
145.80	201.0
148.00	272.0
149.90	216.0
155.00	255.0
156.80	204.0
159.00	124.0
160.90	155.0
171.10	205.0
172.10	863.0
174.00	85440.0
175.00	6577.0
176.00	82152.0
177.00	5249.0
177.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB251