

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV010620\
 Data File : VV014263.D
 Acq On : 06 Jan 2020 11:11
 Operator : SY/MD
 Sample : VV0106WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK45

Quant Time: Jan 07 01:47:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 07 01:19:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	922810	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	842255	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	379496	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	289469	4.48	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.60%
7) Chloroethane-d5	1.58	69	220179	4.41	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.20%
11) 1,1-Dichloroethene-d2	2.13	63	349824	3.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.40%
20) 2-Butanone-d5	3.96	46	723767	46.66	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.32%
24) Chloroform-d	4.40	84	572263	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
26) 1,2-Dichloroethane-d4	5.08	65	290744	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
32) Benzene-d6	5.10	84	1213073	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.11	67	379266	4.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.40%
41) Toluene-d8	7.36	98	1097447	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
43) trans-1,3-Dichloropropene-	7.66	79	160489	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	8.13	63	660904	45.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.56%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	254664	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	346207	4.86	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.20%


Target Compounds					Qvalue
16) Methylene chloride	2.54	84	12586	0.188 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010620\
Data File : VV014263.D
Acq On : 06 Jan 2020 11:11
Operator : SY/MD
Sample : VV0106WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK45

Quant Time: Jan 07 01:47:34 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 07 01:19:28 2020
Response via : Initial Calibration

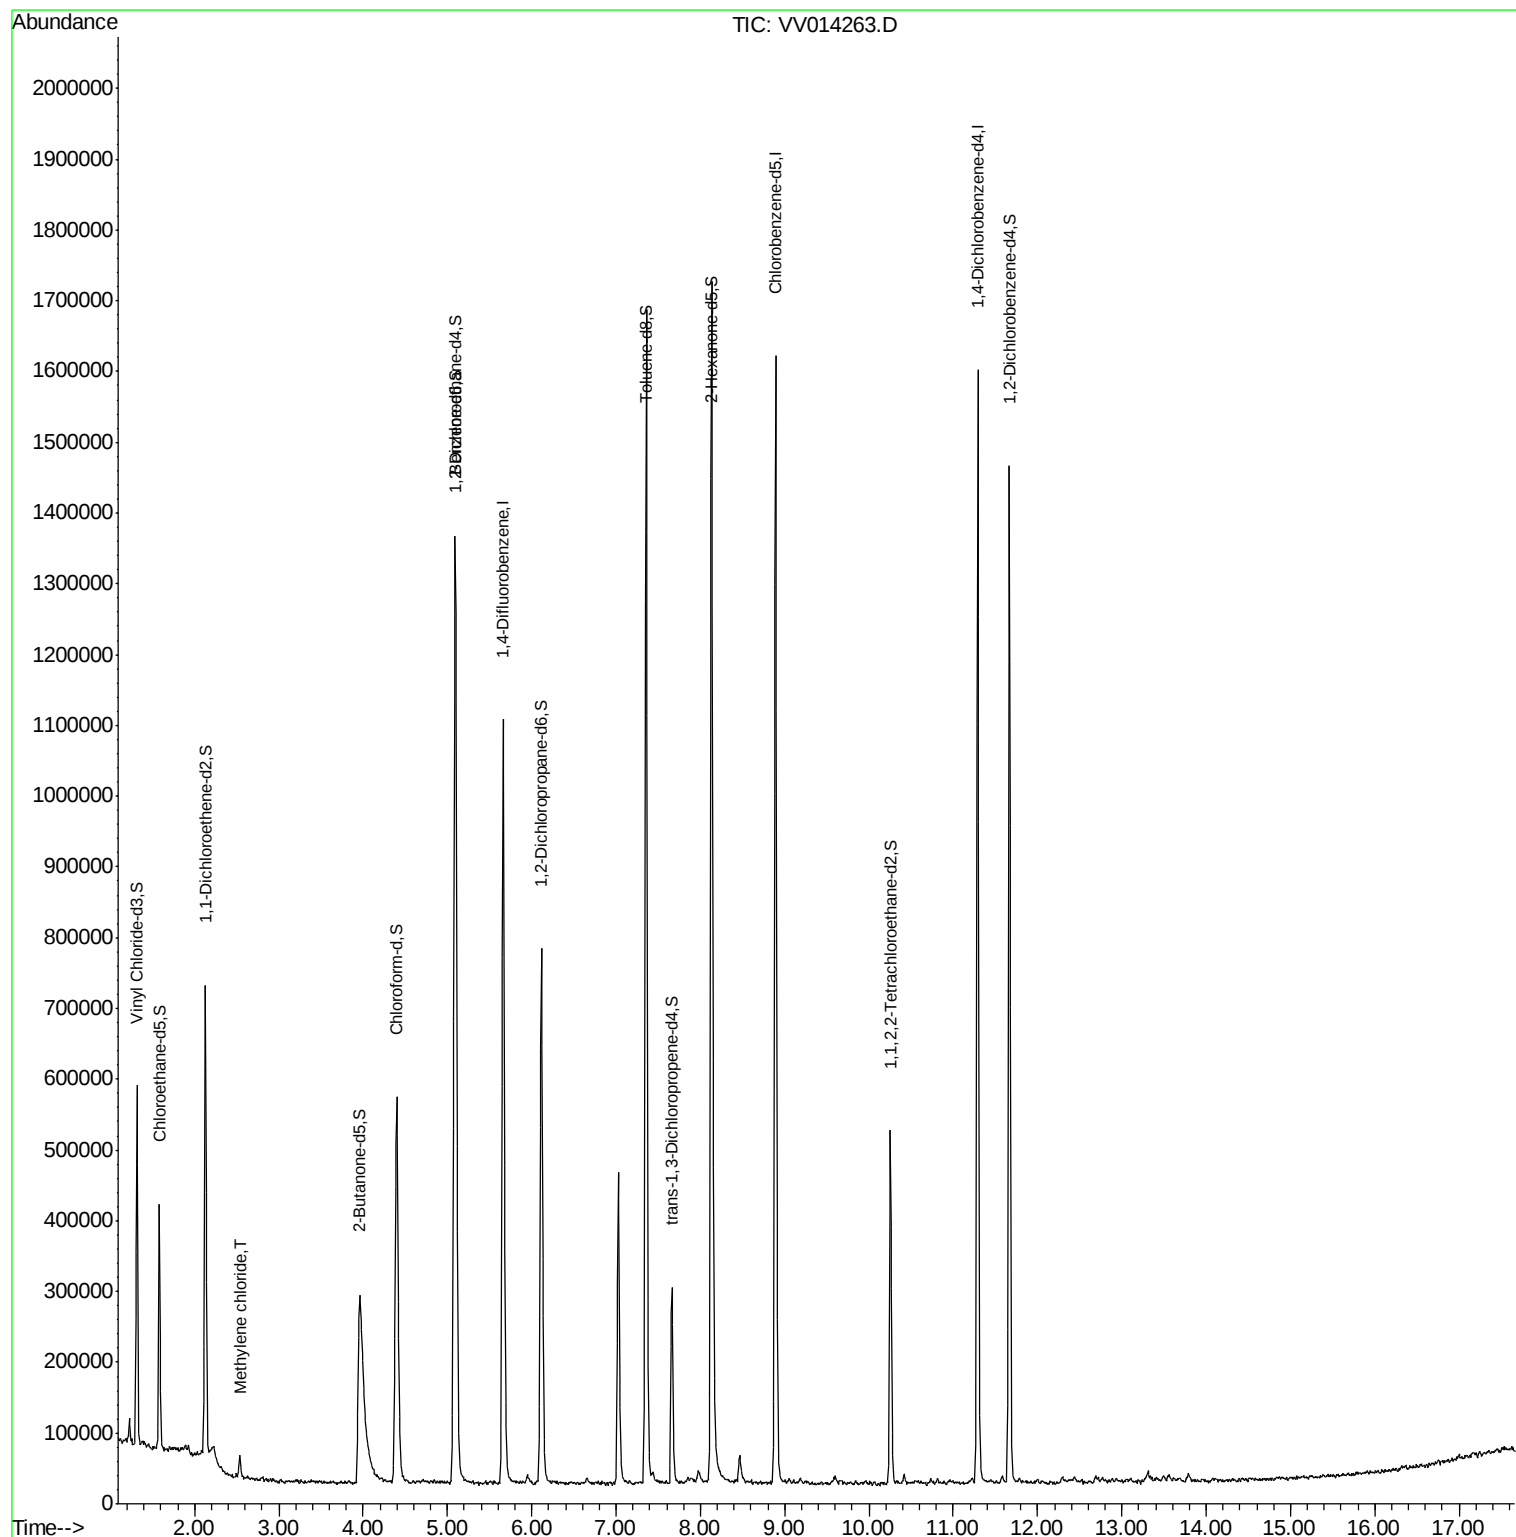

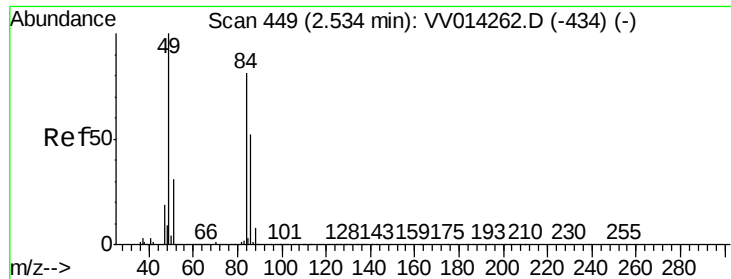

#16
Methylene chloride
Concen: 0.188 ug/L
RT: 2.54 min Scan# 450
Delta R.T. 0.00 min
Lab File: VV014263.D
Acq: 06 Jan 2020 11:11

Instrument :
MSVOA_V
ClientSampleId :
VBLK45

Tgt Ion: 84 Resp: 12586
Ion Ratio Lower Upper
84 100
86 59.6 43.1 80.1
49 137.9 82.1 152.5

