

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV010620\
 Data File : VV014265.D
 Acq On : 06 Jan 2020 12:13
 Operator : SY/MD
 Sample : VIBLK50
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK50

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	80	rBV	496646	486199	14.95%	1.759%
2	1.582	146	153	164	rBV	333728	379012	11.65%	1.371%
3	2.129	313	323	336	rBV	661791	927283	28.51%	3.355%
4	2.537	440	450	462	rBV	158233	267952	8.24%	0.969%
5	3.968	879	895	933	rBV	225636	1086754	33.42%	3.932%
6	4.399	1012	1029	1059	rBV	545214	1347306	41.43%	4.874%
7	5.093	1228	1245	1274	rBV2	1365801	3252157	100.00%	11.766%
8	5.659	1409	1421	1444	rBV	1193919	2352602	72.34%	8.511%
9	6.116	1550	1563	1588	rBV	743177	1505638	46.30%	5.447%
10	7.026	1834	1846	1868	rBV	448334	809925	24.90%	2.930%
11	7.357	1936	1949	1965	rBV	1666195	2875388	88.41%	10.403%
12	7.662	2033	2044	2059	rBV	269914	474012	14.58%	1.715%
13	7.978	2131	2142	2151	rBV	25164	50403	1.55%	0.182%
14	8.132	2179	2190	2224	rBV	1635820	3155280	97.02%	11.415%
15	8.891	2414	2426	2444	rBV	1731523	2801478	86.14%	10.135%
16	10.257	2837	2851	2870	rBV	506914	815583	25.08%	2.951%
17	10.421	2890	2902	2911	rVB3	23898	42621	1.31%	0.154%
18	11.289	3160	3172	3189	rBV	1715145	2651920	81.54%	9.594%
19	11.575	3252	3261	3277	rBV2	96289	172877	5.32%	0.625%
20	11.666	3277	3289	3310	rVB	1383164	2186023	67.22%	7.909%


Sum of corrected areas: 27640413

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010620\
Data File : VV014265.D
Acq On : 06 Jan 2020 12:13
Operator : SY/MD
Sample : VIBLK50
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

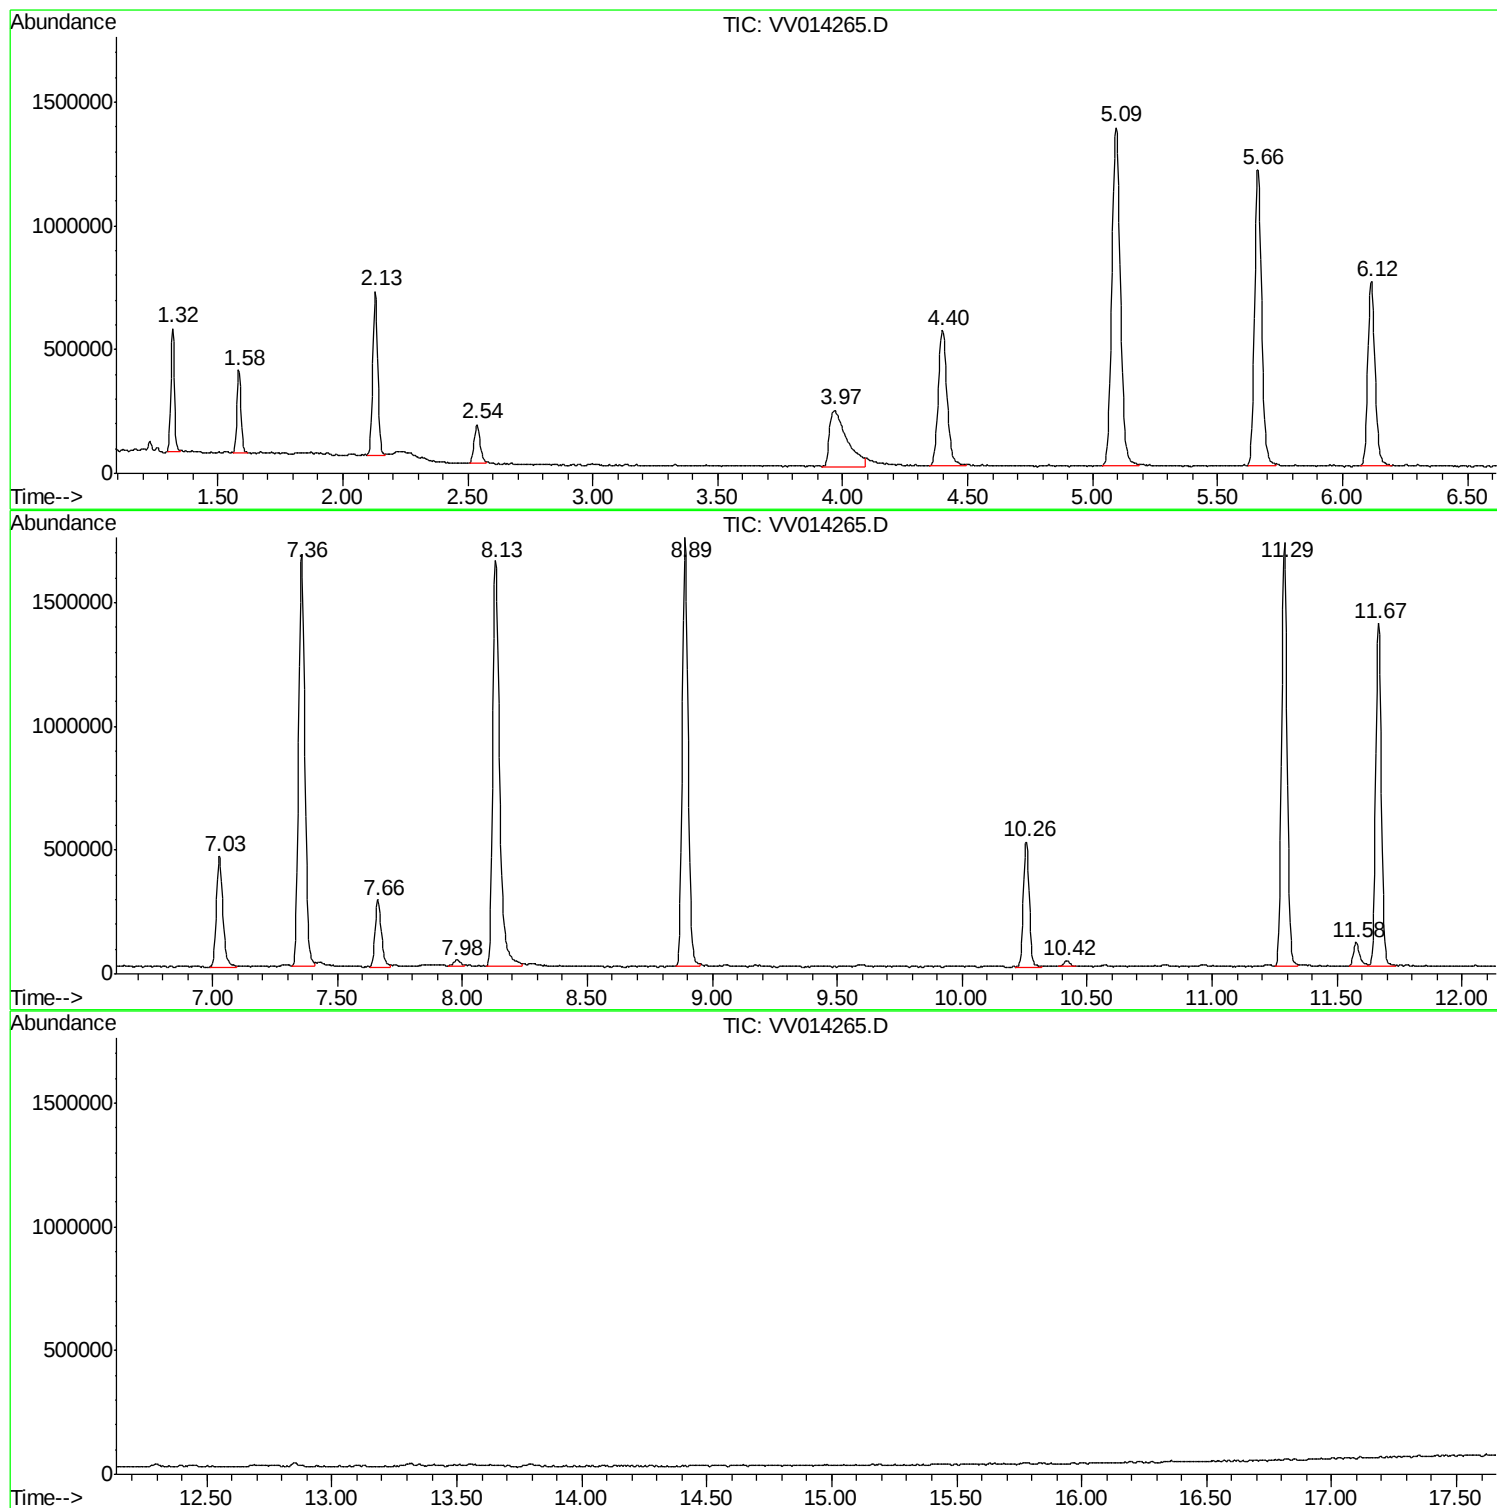

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV010620\
Data File : VV014265.D
Acq On : 06 Jan 2020 12:13
Operator : SY/MD
Sample : VIBLK50
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK50

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV010620\
Data File : VV014265.D
Acq On : 06 Jan 2020 12:13
Operator : SY/MD
Sample : VIBLK50
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK50

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc