

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010621\
 Data File : VV019908.D
 Acq On : 06 Jan 2021 13:12
 Operator : SY/MD
 Sample : VV0106WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jan 07 06:36:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM010621.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jan 07 06:31:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	8553	0.50	ug/L	# 0.00
5) Chlorobenzene-d5	8.863	117	8021	0.50	ug/L	# 0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	3989	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	3397	0.47	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	94.00%		
4) 1,2-Dichloroethane-d4	5.042	65	3404	0.48	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.00%		
7) 1,2-Dichloropropane-d6	6.068	67	4175	0.51	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	102.00%		
8) Toluene-d8	7.317	98	9105	0.49	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.00%		
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2395	0.49	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.00%		
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.426	75	15	0.02	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010621\
Data File : VV019908.D
Acq On : 06 Jan 2021 13:12
Operator : SY/MD
Sample : VV0106WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jan 07 06:36:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM010621.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jan 07 06:31:40 2021
Response via : Initial Calibration

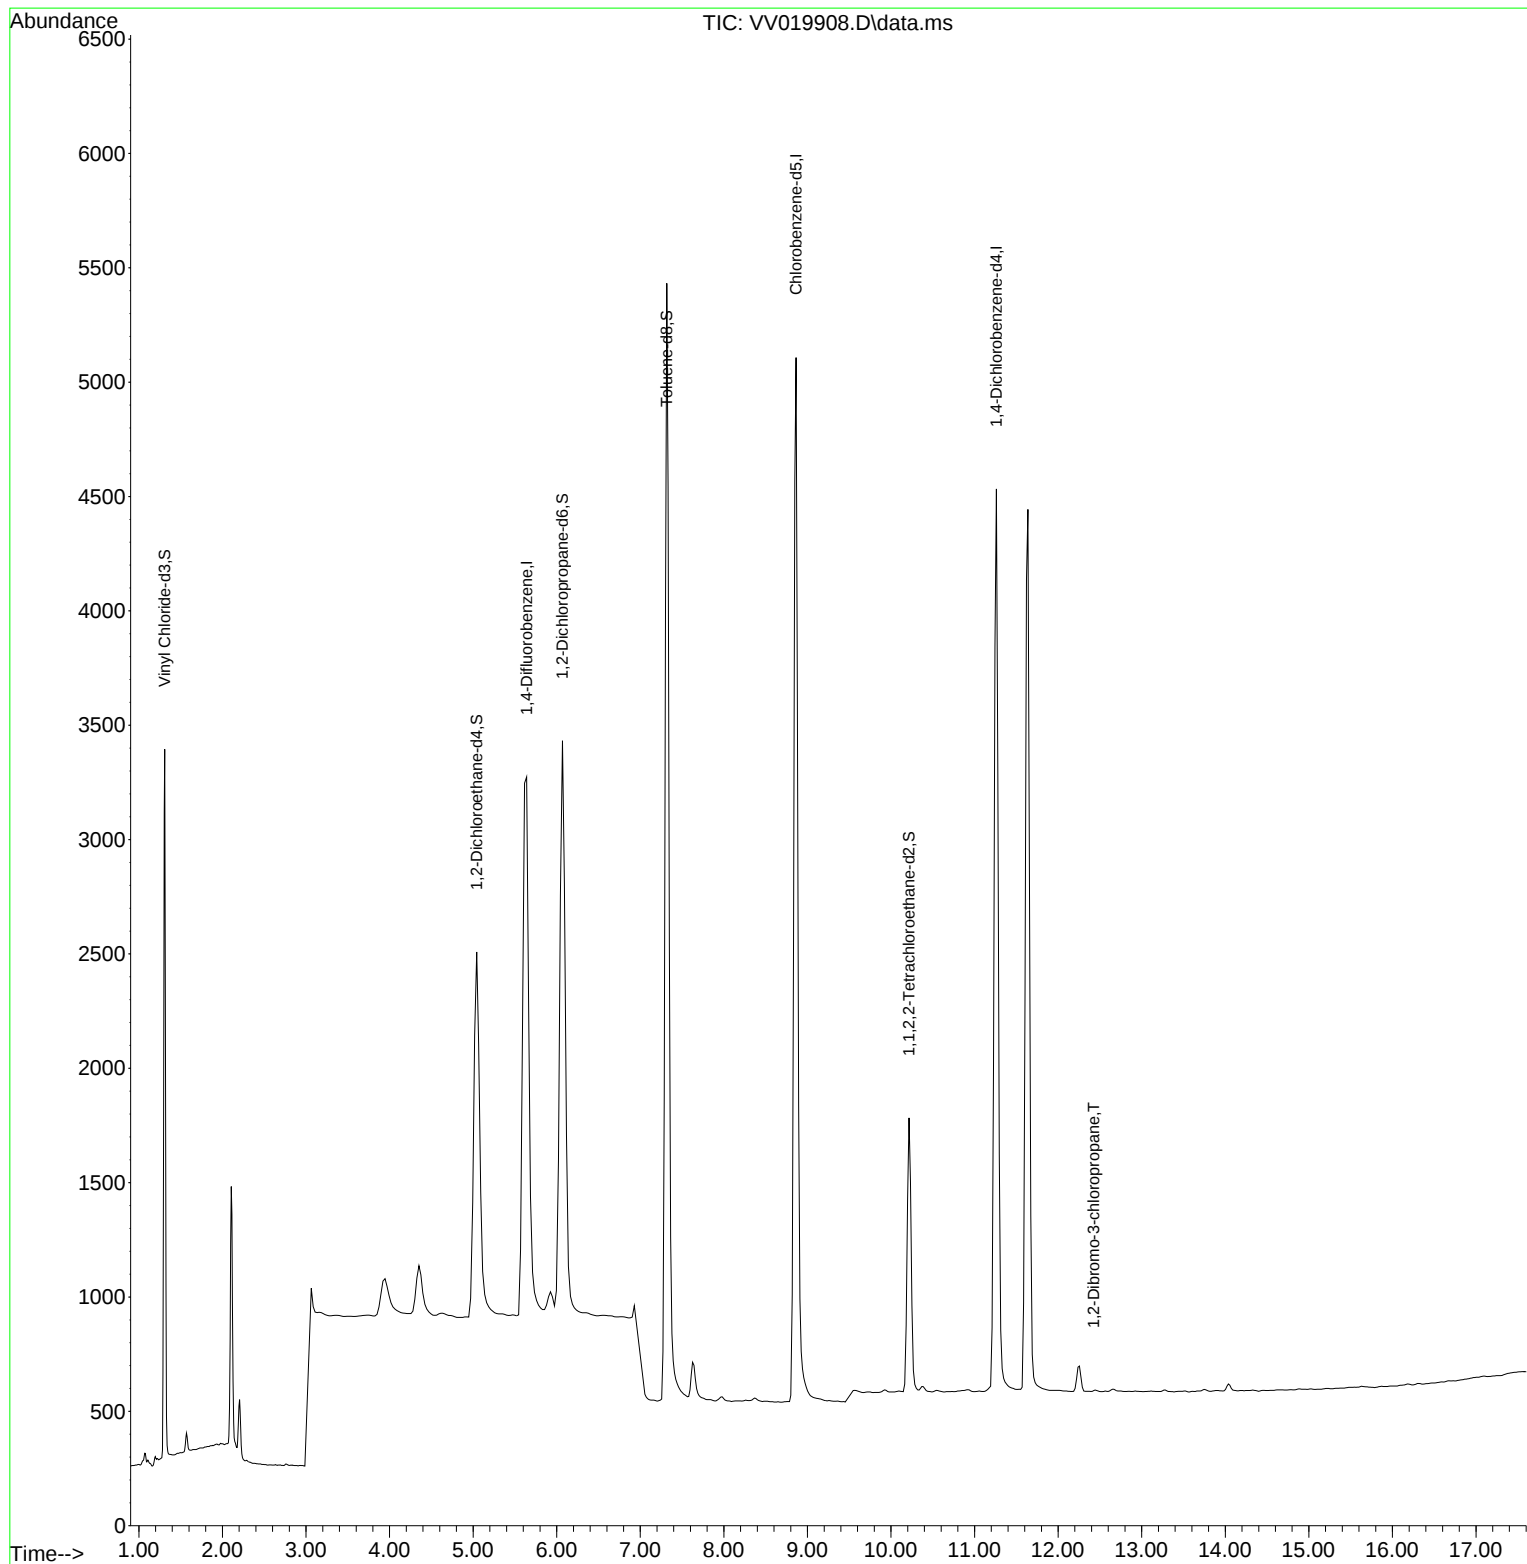

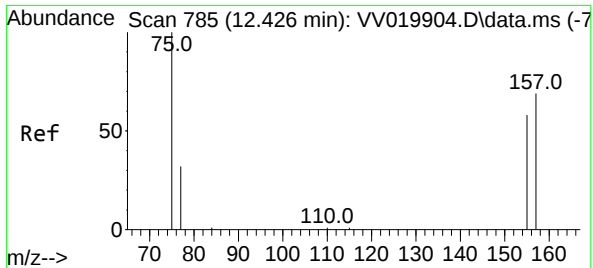

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.02 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV019908.D
 Acq: 06 Jan 2021 13:12

Instrument :
 MSVOA_V
 ClientSampleId :

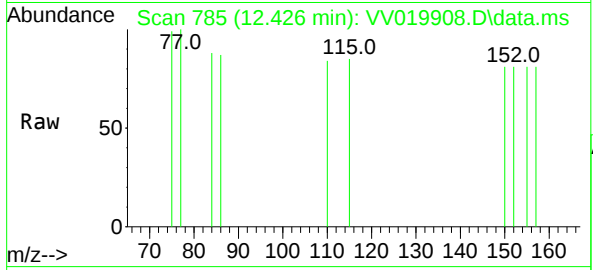

Tgt Ion:	75	Resp:	15
Ion	Ratio	Lower	Upper
75	100		
157	82.1	60.6	90.8
155	82.1	55.8	83.6

