


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010621\
 Data File : VV019901.D
 Acq On : 06 Jan 2021 09:50
 Operator : SY/MD
 Sample : BFB32
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB200

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM010621.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jan 07 18:16:53 2021

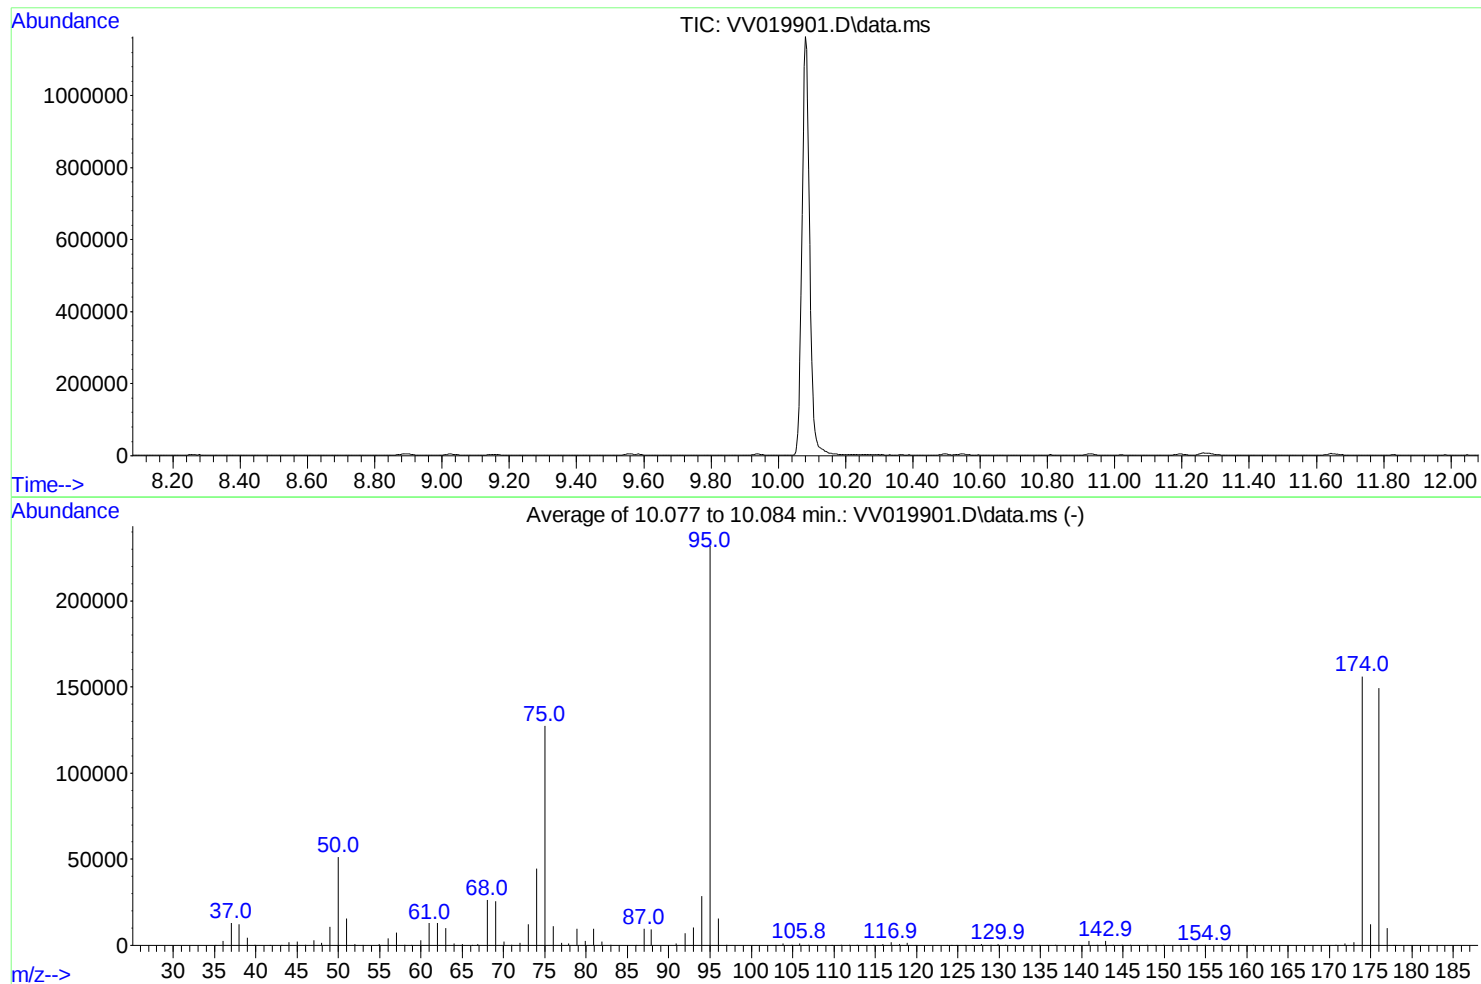

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2782

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	51283	PASS
75	95	30	80	55.0	127501	PASS
95	95	100	100	100.0	231680	PASS
96	95	5	9	6.8	15681	PASS
173	174	0.00	2	1.3	2015	PASS
174	95	50	120	67.4	156160	PASS
175	174	5	9	7.9	12325	PASS
176	174	95	101	95.5	149141	PASS
177	176	5	9	6.8	10127	PASS

m/z	Abundance
35.70	156.0
39.00	143.0
39.90	242.0
41.10	133.0
42.70	116.0
44.00	691.0
45.20	100.0
105.30	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200

m/z	Abundance
36.00	2536.0
37.00	13024.0
38.00	11698.0
39.00	4697.0
40.00	464.0
42.60	143.0
43.10	125.0
44.00	2369.0
45.00	2161.0
46.00	420.0
47.00	3052.0
48.00	1613.0
49.00	10775.0
50.00	50648.0
51.00	15268.0
52.00	815.0
53.00	164.0
54.90	850.0
56.00	4205.0
57.00	7021.0
58.00	412.0
58.80	107.0
60.00	2617.0
61.00	12318.0
62.00	12993.0
63.00	9773.0
64.00	1158.0
65.00	789.0
66.80	551.0
68.00	25304.0
69.00	25280.0
70.00	1971.0
71.00	178.0
72.00	1420.0
73.00	11952.0
74.00	43488.0
75.00	123360.0
76.00	10657.0
77.00	1554.0
77.90	1000.0
78.90	9659.0
79.90	2543.0
80.90	9599.0
81.90	2161.0
83.00	268.0
87.00	9818.0
87.90	9045.0
90.90	1027.0
92.00	6622.0
93.00	9922.0
94.00	27936.0
95.00	223360.0
96.00	15349.0
97.00	399.0
102.90	147.0
103.90	1032.0
104.90	353.0
105.90	1159.0
106.90	277.0
109.70	159.0
110.80	288.0
111.90	236.0
112.80	291.0
114.80	345.0
115.90	906.0
116.90	1763.0
118.00	754.0
118.90	1470.0
123.70	170.0
124.30	104.0
124.80	101.0
125.80	148.0
126.80	129.0
127.80	679.0
129.00	451.0
129.90	747.0
130.80	396.0
134.90	445.0
136.80	380.0
139.70	169.0
140.90	2349.0
141.90	375.0
142.90	2536.0
143.90	210.0
144.90	406.0
146.00	362.0
146.80	141.0
147.90	410.0
148.90	144.0
150.00	240.0
152.70	149.0
153.10	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200

153.90	130.0
154.90	463.0
156.90	390.0
158.10	110.0
159.00	245.0
160.80	248.0
170.80	224.0
171.90	965.0
173.00	1875.0
174.00	146432.0
175.00	11947.0
175.90	139456.0
177.00	9958.0
177.80	232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200

m/z	Abundance
36.00	2767.0
37.00	13643.0
38.00	12560.0
39.00	4713.0
40.00	496.0
41.60	134.0
42.60	122.0
43.10	152.0
44.00	2679.0
45.00	2352.0
46.00	411.0
47.00	3334.0
47.90	1493.0
49.00	11228.0
50.00	53024.0
51.00	16286.0
52.00	904.0
52.90	167.0
54.90	954.0
56.00	4392.0
57.00	7848.0
58.00	409.0
60.00	2936.0
61.00	13261.0
62.00	13307.0
63.00	10430.0
64.00	1245.0
65.00	920.0
66.20	127.0
66.90	690.0
68.00	27008.0
69.00	26536.0
70.10	2210.0
71.00	217.0
72.00	1513.0
73.00	12739.0
74.00	46176.0
75.00	132096.0
76.00	11473.0
77.00	1631.0
77.90	996.0
78.90	10158.0
79.90	2479.0
80.90	10145.0
81.90	2303.0
82.90	244.0
86.00	263.0
87.00	10099.0
87.90	9873.0
90.90	1198.0
92.00	7454.0
93.00	10793.0
94.00	29696.0
95.00	239936.0
96.00	16191.0
97.00	387.0
102.90	170.0
103.90	987.0
104.90	404.0
105.80	1253.0
106.90	318.0
109.80	189.0
110.80	243.0
111.90	226.0
112.80	265.0
114.90	420.0
115.90	871.0
116.90	1838.0
118.00	766.0
118.90	1523.0
123.70	124.0
124.80	104.0
125.80	133.0
126.80	128.0
127.90	720.0
129.00	529.0
129.90	885.0
130.80	418.0
134.90	457.0
135.80	105.0
136.90	424.0
139.00	121.0
139.70	179.0
140.90	2586.0
141.90	371.0
142.90	2625.0
143.80	263.0
144.90	419.0
146.00	364.0
146.80	114.0
147.90	459.0
148.80	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200

149.90	239.0
152.90	198.0
153.00	196.0
153.80	143.0
155.00	482.0
156.90	449.0
159.00	310.0
160.80	266.0
169.70	104.0
170.80	252.0
171.90	1065.0
173.00	2066.0
174.00	161920.0
175.00	12848.0
175.90	154304.0
177.00	10538.0
178.00	262.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200

m/z	Abundance
35.10	111.0
36.00	2596.0
37.00	12909.0
38.00	12188.0
39.00	4295.0
39.90	540.0
41.70	140.0
43.00	153.0
44.00	2701.0
45.00	2272.0
46.00	352.0
47.00	3104.0
47.90	1328.0
49.00	10441.0
50.00	50176.0
51.00	15543.0
52.00	803.0
52.90	159.0
54.90	899.0
56.00	4150.0
57.00	7657.0
58.00	377.0
60.00	2901.0
61.00	12937.0
62.00	12268.0
63.00	9944.0
64.00	1132.0
65.00	911.0
66.90	826.0
68.00	26728.0
69.00	25128.0
70.10	2240.0
71.00	204.0
72.00	1515.0
73.00	11952.0
74.00	44256.0
75.00	127048.0
76.00	11238.0
77.00	1589.0
77.90	923.0
78.90	9394.0
79.90	2396.0
80.90	9784.0
81.90	2329.0
82.90	185.0
86.00	293.0
87.00	9630.0
87.90	9485.0
90.90	1261.0
92.00	7398.0
93.00	10801.0
94.00	28728.0
95.00	231744.0
96.00	15504.0
97.00	328.0
102.90	170.0
103.80	888.0
104.90	393.0
105.90	1207.0
106.90	258.0
109.80	226.0
110.90	228.0
111.90	181.0
112.80	225.0
114.90	392.0
115.90	847.0
116.90	1833.0
117.90	809.0
118.90	1347.0
119.90	104.0
124.10	123.0
124.80	114.0
125.90	105.0
126.80	107.0
127.90	771.0
129.00	484.0
129.90	1000.0
130.80	402.0
134.90	444.0
135.80	113.0
136.90	452.0
139.00	130.0
139.80	144.0
140.90	2574.0
141.90	323.0
142.90	2563.0
143.80	258.0
144.90	392.0
145.80	321.0
147.90	534.0
148.80	237.0
149.90	227.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200

151.90	149.0
152.90	216.0
153.80	145.0
154.90	452.0
156.90	501.0
159.00	324.0
160.80	284.0
169.80	138.0
170.80	240.0
171.90	1124.0
173.00	2104.0
174.00	160128.0
175.00	12180.0
176.00	153664.0
177.00	9884.0
178.00	324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB200