




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
 Data File : VV024295.D
 Acq On : 06 Jan 2022 15:03
 Operator : SY/MD
 Sample : N1053-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH8

Manual IntegrationsAPPROVED

Quant Time: Jan 07 01:38:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 07 01:34:41 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 01/07/2022
 Supervised By :Amit Patel 01/07/2022

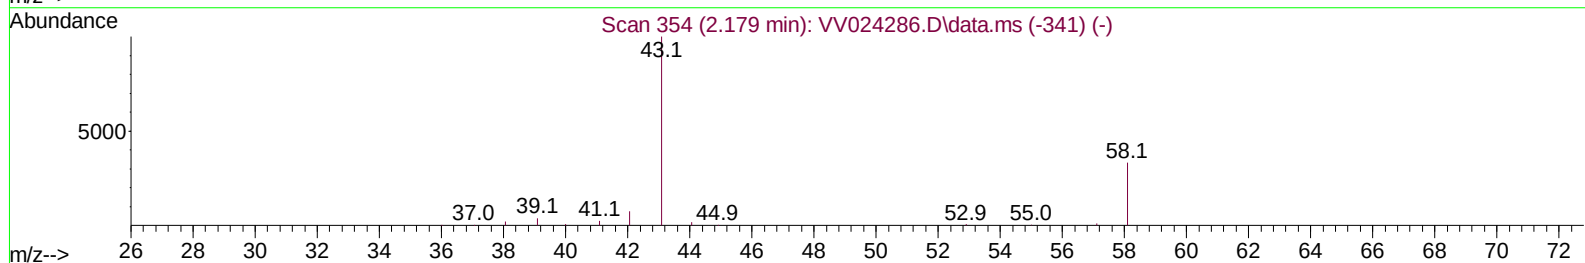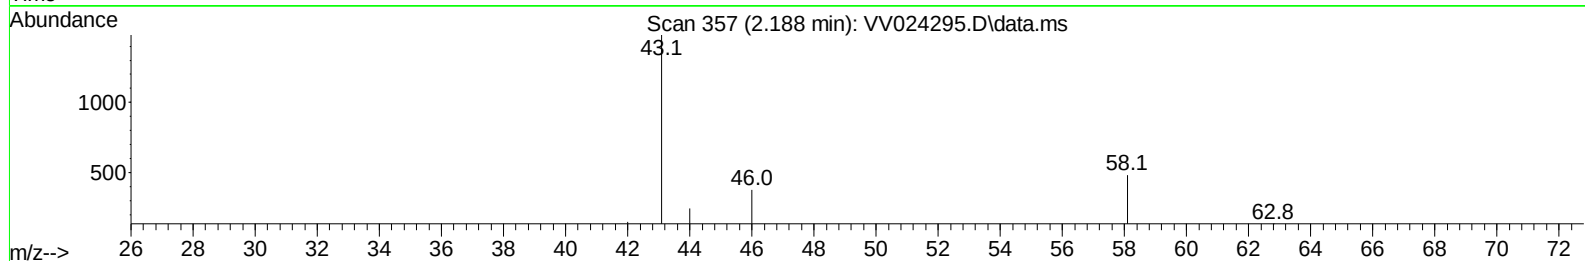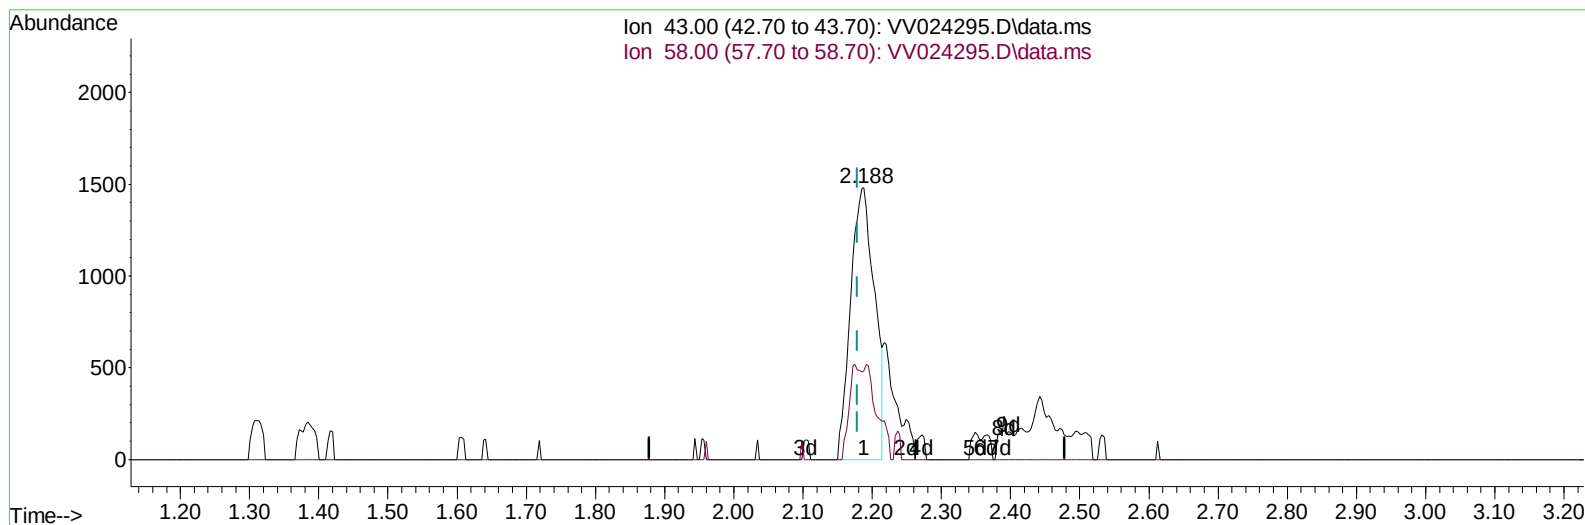

TIC: VV024295.D\data.ms

(13) Acetone (T)

2.188min (+ 0.010) 3.90 ug/L

response 3546

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.50	18.39
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
Data File : VV024295.D
Acq On : 06 Jan 2022 15:03
Operator : SY/MD
Sample : N1053-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLH8

Manual IntegrationsAPPROVED

Quant Time: Jan 07 01:38:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 07 01:34:41 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 01/07/2022
Supervised By :Amit Patel 01/07/2022

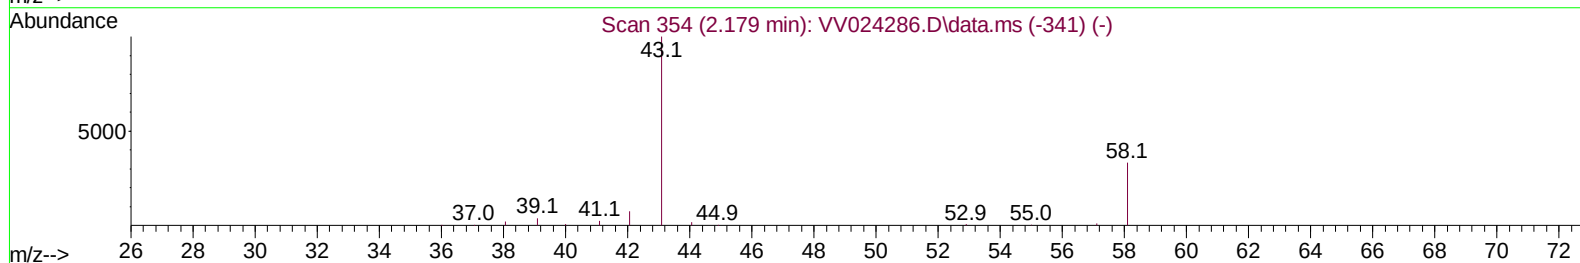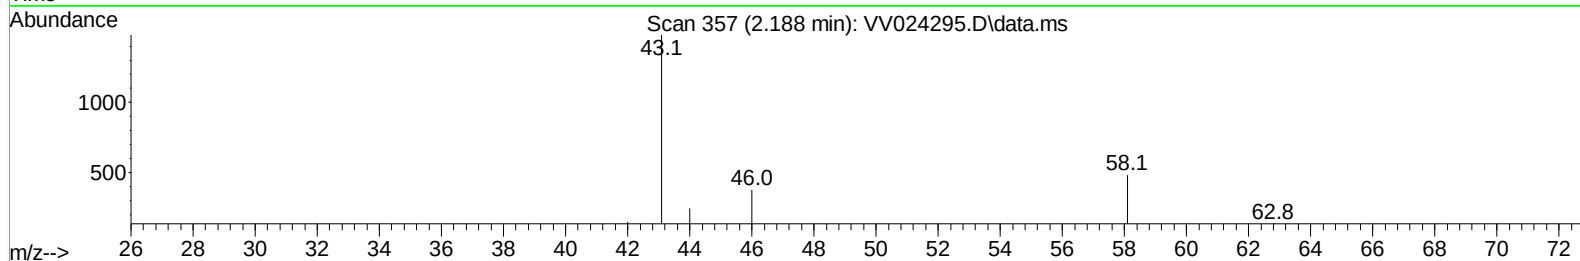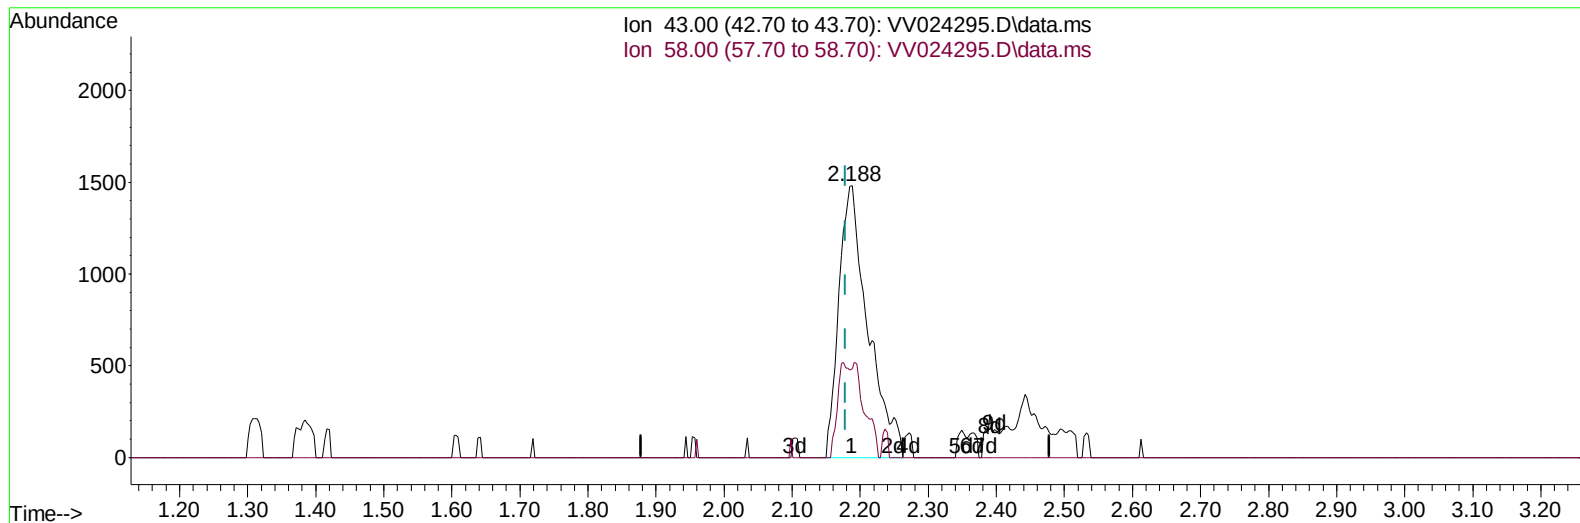

TIC: VV024295.D\data.ms

(13) Acetone (T)

2.188min (+ 0.010) 4.83 ug/L m

response 4399

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.50	14.82
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
 Data File : VV024295.D
 Acq On : 06 Jan 2022 15:03
 Operator : SY/MD
 Sample : N1053-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH8

Manual IntegrationsAPPROVED

Quant Time: Jan 07 01:38:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 07 01:34:41 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 01/07/2022
 Supervised By :Amit Patel 01/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	229911	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	216941	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	108816	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	65234	39.425	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	78.840%	
7) Chloroethane-d5	1.571	69	54318	43.214	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	86.420%	
11) 1,1-Dichloroethene-d2	2.111	63	101978	32.976	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	65.960%	
21) 2-Butanone-d5	3.889	46	80905	87.762	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	87.760%	
24) Chloroform-d	4.349	84	135038	44.654	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	89.300%	
26) 1,2-Dichloroethane-d4	5.031	65	92782	45.825	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.640%	
32) Benzene-d6	5.050	84	256599	45.326	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.660%	
36) 1,2-Dichloropropane-d6	6.069	67	71097	44.811	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	89.620%	
41) Toluene-d8	7.317	98	245840	44.851	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	89.700%	
43) trans-1,3-Dichloroprop...	7.622	79	40166	43.964	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	87.920%	
47) 2-Hexanone-d5	8.088	63	54605	79.217	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	79.220%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	92616	40.848	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	81.700%	
66) 1,2-Dichlorobenzene-d4	11.622	152	107318	49.479	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	98.960%	
Target Compounds						
13) Acetone	2.188	43	4399m	4.833	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
Data File : VV024295.D
Acq On : 06 Jan 2022 15:03
Operator : SY/MD
Sample : N1053-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
BGLH8

Manual IntegrationsAPPROVED

Quant Time: Jan 07 01:38:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 07 01:34:41 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 01/07/2022
Supervised By :Amit Patel 01/07/2022

