

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW010622\
 Data File : VW024295.D
 Acq On : 06 Jan 2022 15:03
 Operator : SY/MD
 Sample : N1053-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH8

Quant Time: Jan 07 01:38:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 07 01:34:41 2022
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 01/07/2022
 Supervised By :Amit Patel 01/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	229911	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	216941	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	108816	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	65234	39.425	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.840%		
7) Chloroethane-d5	1.571	69	54318	43.214	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.420%		
11) 1,1-Dichloroethene-d2	2.111	63	101978	32.976	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.960%		
21) 2-Butanone-d5	3.889	46	80905	87.762	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.760%		
24) Chloroform-d	4.349	84	135038	44.654	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.300%		
26) 1,2-Dichloroethane-d4	5.031	65	92782	45.825	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.640%		
32) Benzene-d6	5.050	84	256599	45.326	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.660%		
36) 1,2-Dichloropropane-d6	6.069	67	71097	44.811	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.620%		
41) Toluene-d8	7.317	98	245840	44.851	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.700%		
43) trans-1,3-Dichloroprop...	7.622	79	40166	43.964	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.920%		
47) 2-Hexanone-d5	8.088	63	54605	79.217	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	79.220%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	92616	40.848	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.700%		
66) 1,2-Dichlorobenzene-d4	11.622	152	107318	49.479	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.960%		
Target Compounds						
13) Acetone	2.188	43	4399m	4.833	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
Data File : VV024295.D
Acq On : 06 Jan 2022 15:03
Operator : SY/MD
Sample : N1053-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BGLH8

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 01/07/2022
Supervised By :Amit Patel 01/07/2022


Quant Time: Jan 07 01:38:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 07 01:34:41 2022
Response via : Initial Calibration

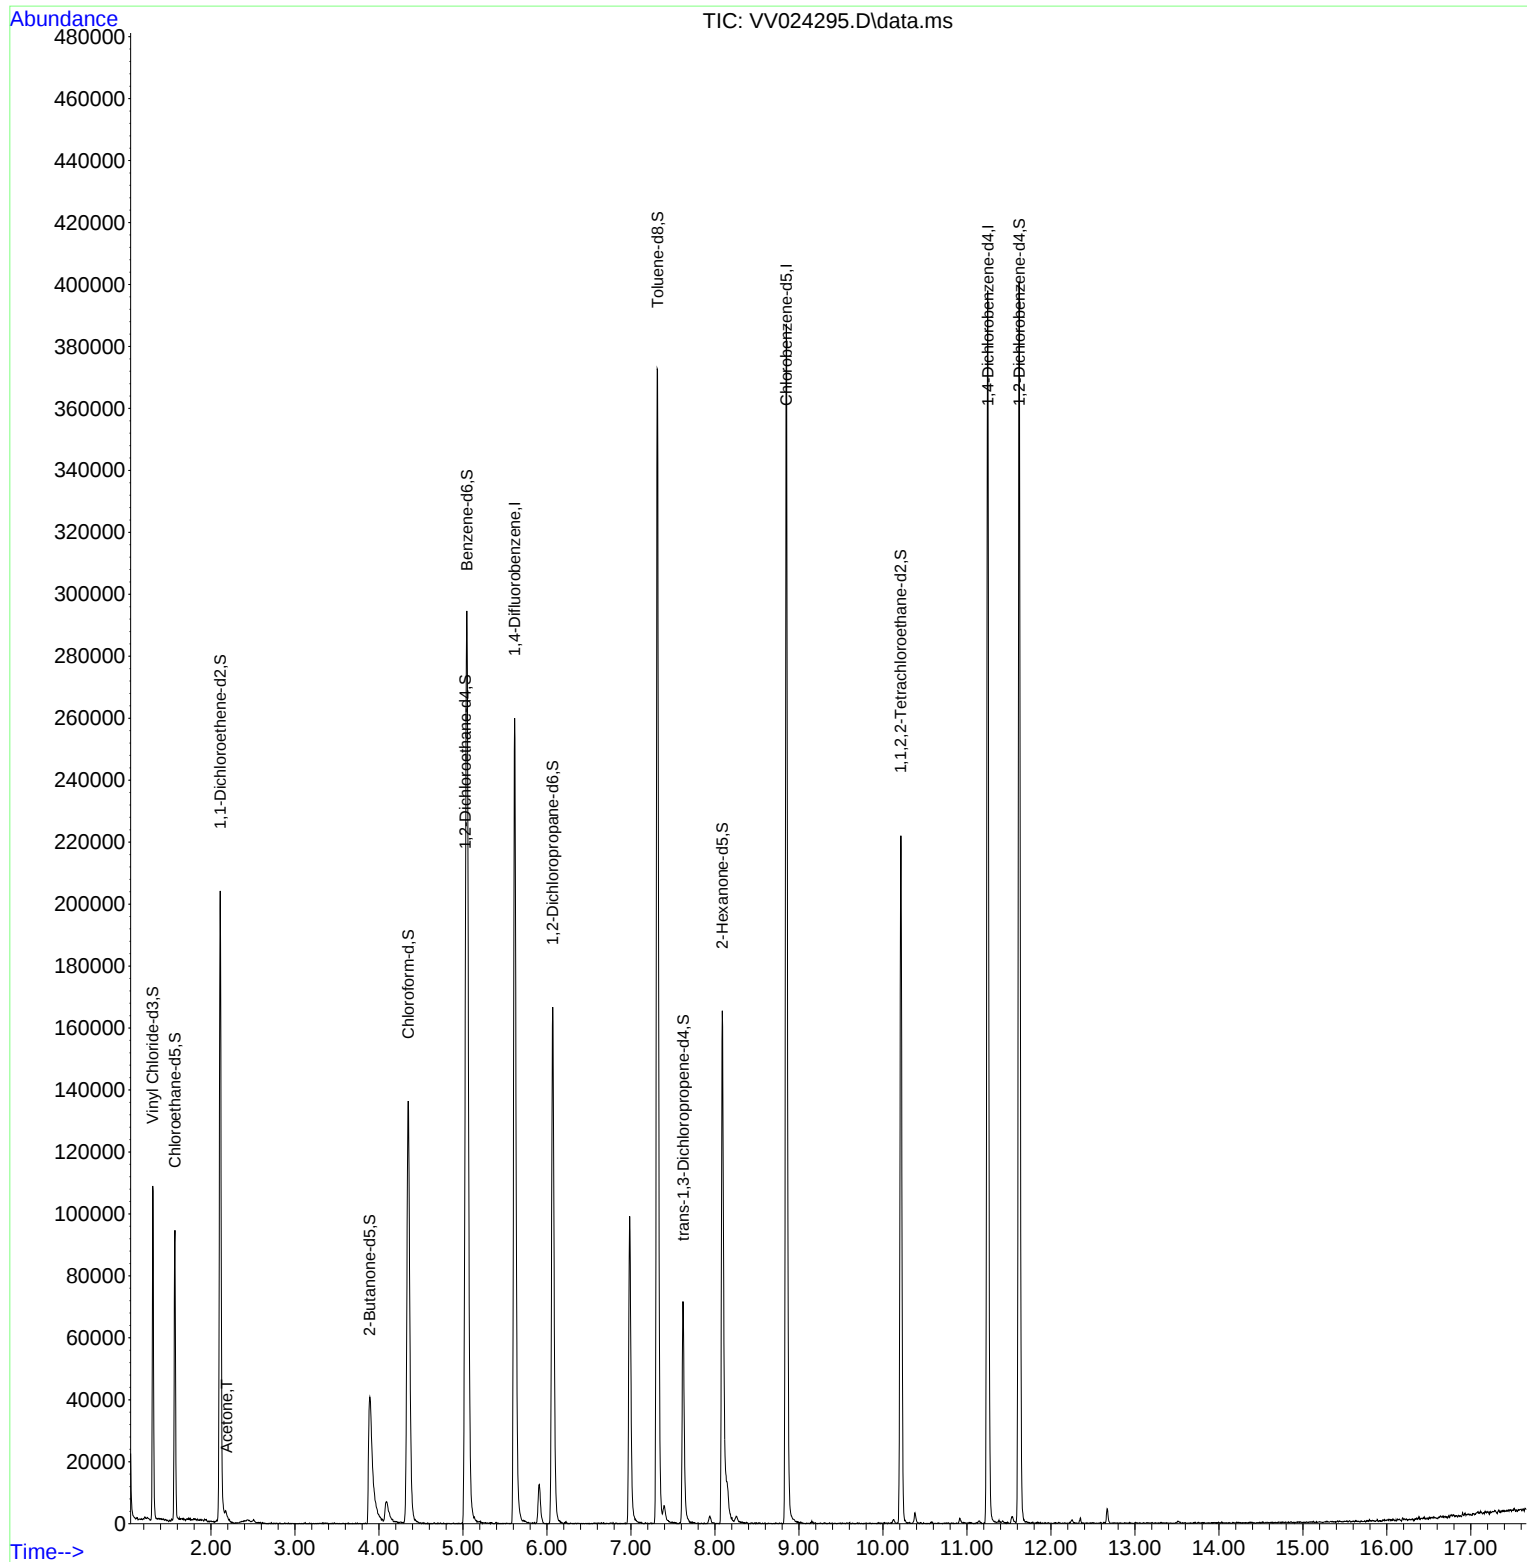

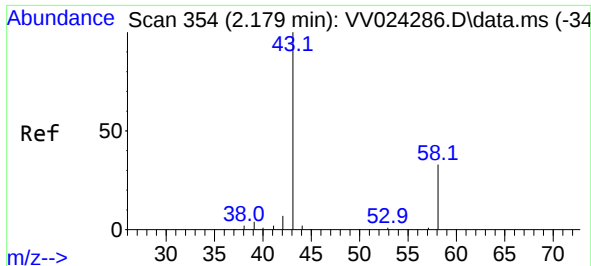

#13
Acetone
Concen: 4.833 ug/L m
RT: 2.188 min Scan# 31
Delta R.T. 0.010 min
Lab File: VV024295.D
Acq: 06 Jan 2022 15:03

Instrument :
MSVOA_V
ClientSampleId :
BGLH8

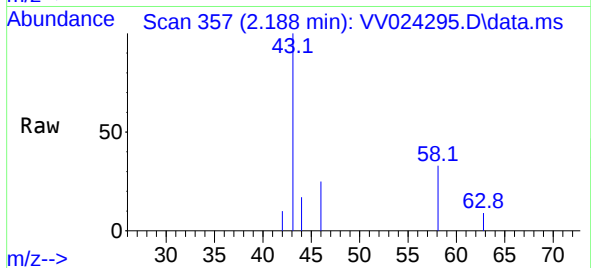

Tgt Ion: 43 Resp: 4399
Ion Ratio Lower Upper
43 100
58 14.8 0.0 63.0

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 01/07/2022
Supervised By :Amit Patel 01/07/2022

