

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW010622\
 Data File : VW024298.D
 Acq On : 06 Jan 2022 16:14
 Operator : SY/MD
 Sample : N1053-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH9

Quant Time: Jan 07 01:39:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 07 01:34:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	224750	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	210120	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	103533	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	65311	40.378	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.760%
7) Chloroethane-d5	1.568	69	52550	42.767	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.540%
11) 1,1-Dichloroethene-d2	2.108	63	99367	32.870	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.740%
21) 2-Butanone-d5	3.886	46	78547	87.160	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.160%
24) Chloroform-d	4.349	84	133106	45.026	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.060%
26) 1,2-Dichloroethane-d4	5.031	65	89844	45.393	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.780%
32) Benzene-d6	5.050	84	252173	45.990	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.980%
36) 1,2-Dichloropropane-d6	6.069	67	72347	47.079	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.160%
41) Toluene-d8	7.317	98	239483	45.109	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.220%
43) trans-1,3-Dichloroprop...	7.622	79	38718	43.755	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.520%
47) 2-Hexanone-d5	8.088	63	57254	85.757	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.760%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	96352	43.875	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.740%
66) 1,2-Dichlorobenzene-d4	11.622	152	103206	50.011	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.020%
Target Compounds						
					Qvalue	
46) Tetrachloroethene	7.979	164	7815	5.828	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
Data File : VV024298.D
Acq On : 06 Jan 2022 16:14
Operator : SY/MD
Sample : N1053-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGLH9


Quant Time: Jan 07 01:39:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 07 01:34:41 2022
Response via : Initial Calibration

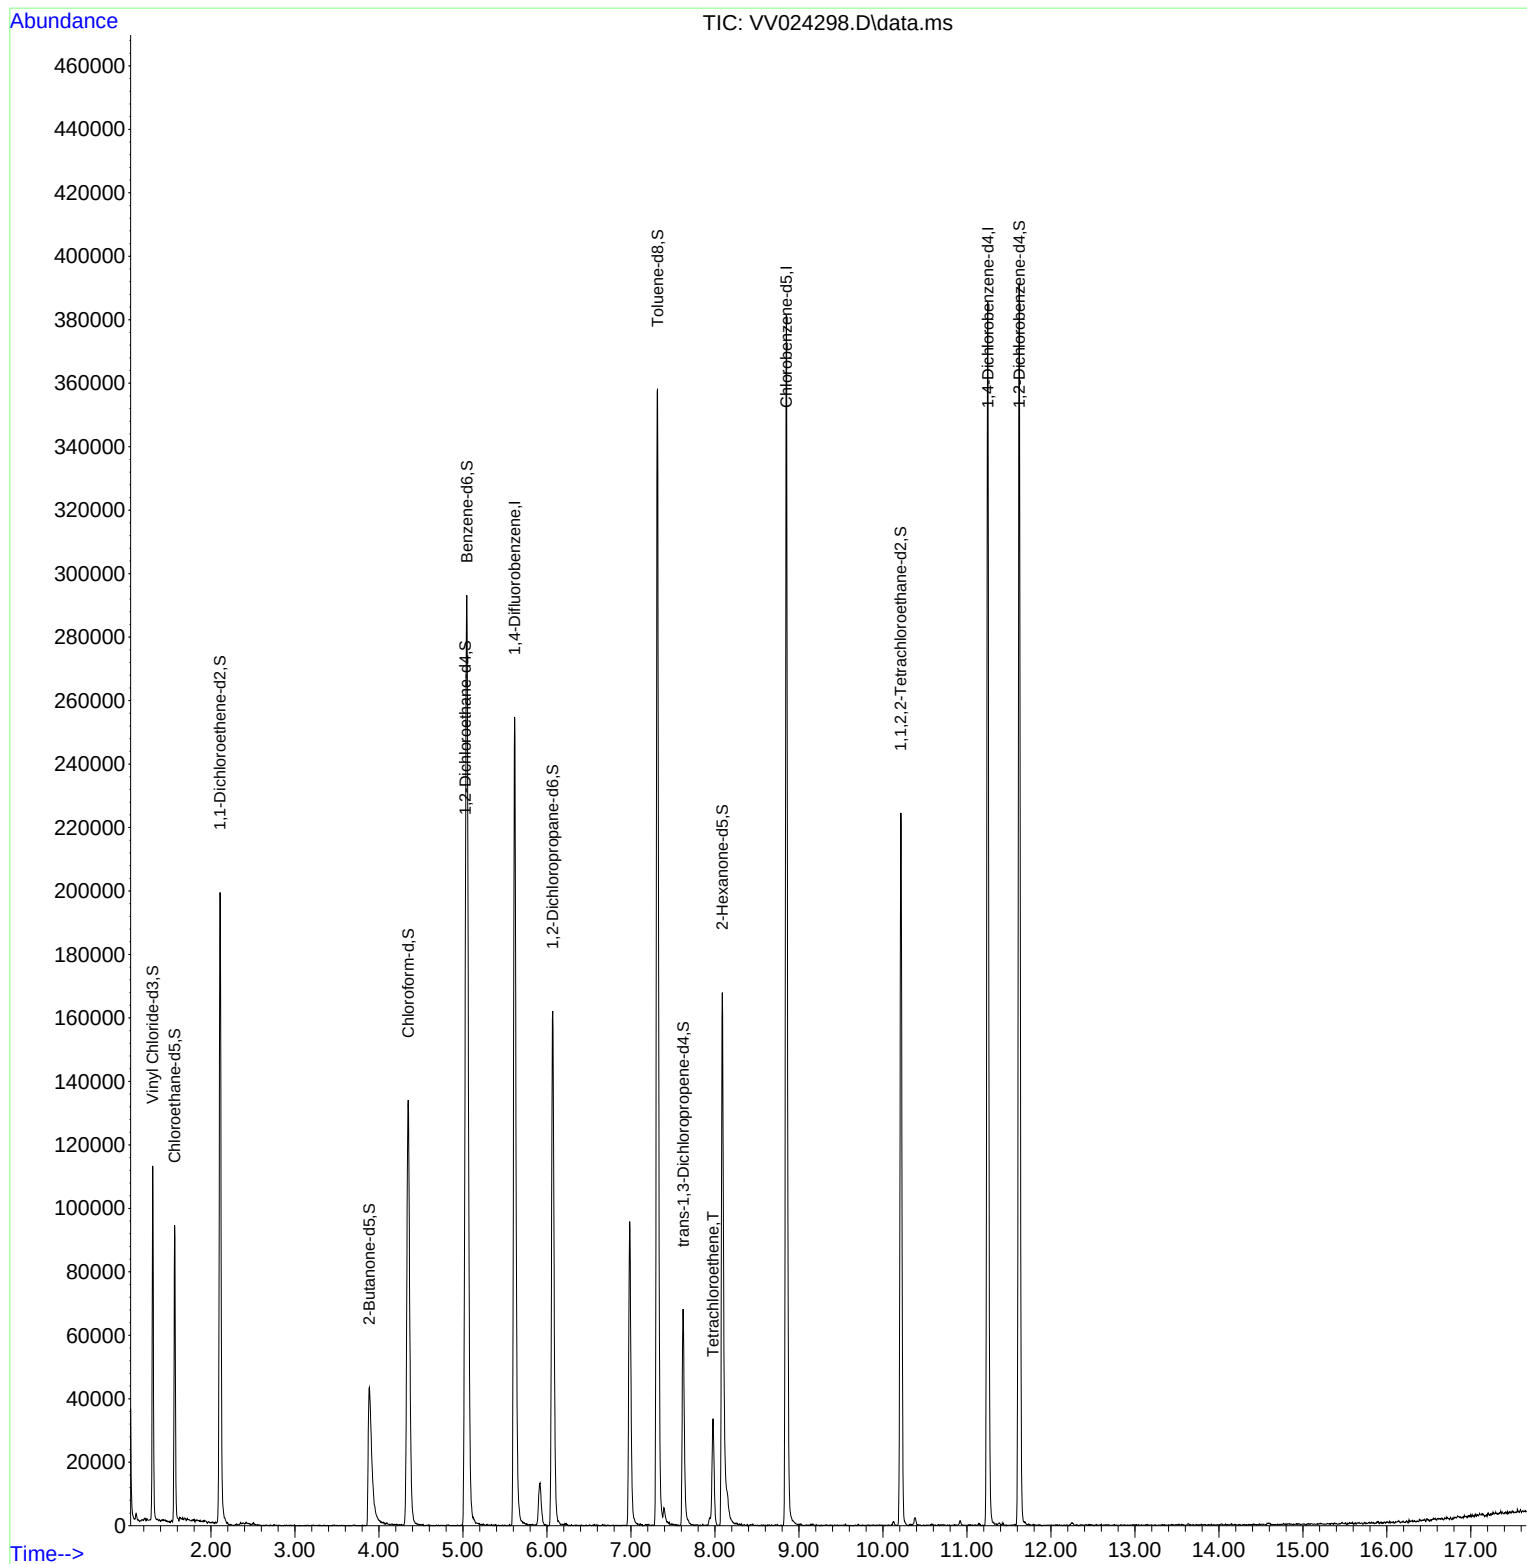

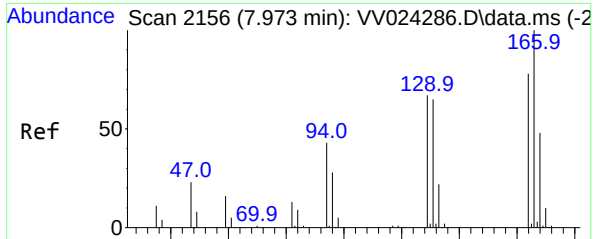

#46
 Tetrachloroethene
 Concen: 5.828 ug/L
 RT: 7.979 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VV024298.D
 Acq: 06 Jan 2022 16:14

Instrument :
 MSVOA_V
 ClientSampleId :
 BGLH9

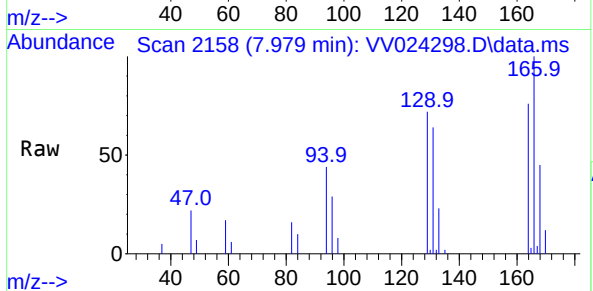

Tgt Ion:164 Resp: 7815

Ion	Ratio	Lower	Upper
164	100		
129	94.5	61.5	114.1
131	84.4	62.2	115.4
166	131.2	89.9	166.9

