

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
 Data File : VV024293.D
 Acq On : 06 Jan 2022 14:14
 Operator : SY/MD
 Sample : N1009-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

Signal : TIC: VV024293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	95	rBV	116117	117103	14.08%	1.793%
2	1.571	158	165	175	rBV	99480	108966	13.10%	1.668%
3	2.111	324	333	356	rVB	219675	321428	38.64%	4.920%
4	2.378	413	416	418	rBV	180	154	0.02%	0.002%
5	2.510	450	457	467	rVB5	2661	3965	0.48%	0.061%
6	2.568	473	475	478	rBV	229	133	0.02%	0.002%
7	2.606	485	487	490	rBV	206	130	0.02%	0.002%
8	2.674	506	508	511	rBB	141	97	0.01%	0.001%
9	2.802	544	548	550	rBB	149	122	0.01%	0.002%
10	2.908	579	581	583	rBB	329	106	0.01%	0.002%
11	2.979	600	603	605	rBV	241	154	0.02%	0.002%
12	3.008	610	612	614	rBB	248	97	0.01%	0.001%
13	3.053	622	626	627	rBB	230	125	0.02%	0.002%
14	3.201	668	672	674	rBV	311	272	0.03%	0.004%
15	3.333	709	713	715	rBV	164	155	0.02%	0.002%
16	3.667	813	817	820	rBB	229	205	0.02%	0.003%
17	3.822	862	865	867	rBB	143	98	0.01%	0.002%
18	3.889	875	886	926	rBV2	48288	148247	17.82%	2.269%
19	4.349	1015	1029	1054	rVB	144559	347391	41.76%	5.318%
20	4.535	1085	1087	1089	rBV	266	153	0.02%	0.002%
21	4.593	1101	1105	1107	rBB	150	97	0.01%	0.001%
22	4.738	1146	1150	1154	rBB2	272	234	0.03%	0.004%
23	4.812	1171	1173	1176	rBB	206	110	0.01%	0.002%
24	4.854	1183	1186	1189	rBB	262	173	0.02%	0.003%
25	4.876	1189	1193	1195	rBB	230	142	0.02%	0.002%
26	4.912	1201	1204	1208	rBB	142	148	0.02%	0.002%
27	4.979	1221	1225	1228	rBB	245	158	0.02%	0.002%
28	5.047	1229	1246	1274	rBV2	318124	831793	100.00%	12.733%
29	5.342	1336	1338	1341	rBV	124	111	0.01%	0.002%
30	5.387	1349	1352	1355	rBB	287	228	0.03%	0.003%
31	5.416	1358	1361	1363	rBB	273	172	0.02%	0.003%
32	5.497	1382	1386	1389	rBB	373	268	0.03%	0.004%
33	5.510	1389	1390	1393	rBV	215	103	0.01%	0.002%
34	5.616	1412	1423	1452	rBV	268231	530883	63.82%	8.127%
35	5.908	1504	1514	1531	rVB4	10398	21533	2.59%	0.330%
36	6.069	1551	1564	1595	rBV	177964	364043	43.77%	5.573%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
 Data File : VV024293.D
 Acq On : 06 Jan 2022 14:14
 Operator : SY/MD
 Sample : N1009-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	6.214	1604	1609	1610	rBV3	851	619	0.07%	0.009%
38	6.336	1644	1647	1649	rBV	292	205	0.02%	0.003%
39	6.426	1673	1675	1678	rBV2	263	167	0.02%	0.003%
40	6.619	1734	1735	1740	rBV	230	187	0.02%	0.003%
41	6.690	1755	1757	1759	rBV	368	175	0.02%	0.003%
42	6.818	1793	1797	1799	rBV	135	142	0.02%	0.002%
43	6.883	1815	1817	1819	rBB	229	127	0.02%	0.002%
44	6.912	1822	1826	1829	rBV2	227	240	0.03%	0.004%
45	6.985	1837	1849	1873	rBV	106884	196332	23.60%	3.005%
46	7.175	1905	1908	1911	rBB	142	118	0.01%	0.002%
47	7.198	1913	1915	1919	rBB2	401	289	0.03%	0.004%
48	7.262	1932	1935	1937	rBV2	250	162	0.02%	0.002%
49	7.313	1940	1951	1972	rBV	396668	687268	82.62%	10.521%
50	7.619	2034	2046	2070	rBV	75208	132922	15.98%	2.035%
51	7.870	2122	2124	2127	rBB	274	169	0.02%	0.003%
52	7.937	2143	2145	2149	rBB	133	110	0.01%	0.002%
53	7.963	2150	2153	2156	rBV2	240	243	0.03%	0.004%
54	8.024	2169	2172	2175	rBV	176	158	0.02%	0.002%
55	8.088	2182	2192	2233	rBV	184082	357184	42.94%	5.468%
56	8.381	2280	2283	2284	rBV	291	182	0.02%	0.003%
57	8.413	2289	2293	2294	rBV	254	209	0.03%	0.003%
58	8.439	2299	2301	2303	rBV	247	139	0.02%	0.002%
59	8.503	2318	2321	2322	rBV	152	108	0.01%	0.002%
60	8.555	2333	2337	2340	rBV	265	262	0.03%	0.004%
61	8.616	2351	2356	2357	rBV	243	181	0.02%	0.003%
62	8.683	2375	2377	2382	rBV	252	240	0.03%	0.004%
63	8.731	2389	2392	2394	rBV	309	224	0.03%	0.003%
64	8.783	2405	2408	2409	rBV	312	178	0.02%	0.003%
65	8.850	2417	2429	2451	rBV	398597	645147	77.56%	9.876%
66	9.063	2493	2495	2496	rBV	237	97	0.01%	0.001%
67	9.117	2509	2512	2514	rBV	222	129	0.02%	0.002%
68	9.191	2532	2535	2537	rBB	148	98	0.01%	0.002%
69	9.207	2537	2540	2542	rBB	155	105	0.01%	0.002%
70	9.294	2565	2567	2570	rBV	140	126	0.02%	0.002%
71	9.342	2580	2582	2585	rBB	152	103	0.01%	0.002%
72	9.371	2588	2591	2592	rBV	160	105	0.01%	0.002%
73	9.442	2610	2613	2616	rBB	249	174	0.02%	0.003%
74	9.497	2627	2630	2633	rBV2	230	198	0.02%	0.003%
75	9.625	2668	2670	2673	rBV	124	109	0.01%	0.002%
76	9.776	2713	2717	2722	rBB2	280	322	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
 Data File : VV024293.D
 Acq On : 06 Jan 2022 14:14
 Operator : SY/MD
 Sample : N1009-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

77	9.837	2734	2736	2737	rBV	223	104	0.01%	0.002%
78	10.018	2789	2792	2794	rBV	151	131	0.02%	0.002%
79	10.040	2796	2799	2800	rBV	162	109	0.01%	0.002%
80	10.079	2808	2811	2812	rBV	281	160	0.02%	0.002%
81	10.124	2820	2825	2832	rBB5	1414	2047	0.25%	0.031%
82	10.156	2832	2835	2836	rBV	178	119	0.01%	0.002%
83	10.214	2842	2853	2879	rBV	245582	382783	46.02%	5.860%
84	10.307	2879	2882	2884	rVB	281	140	0.02%	0.002%
85	10.339	2889	2892	2895	rBV2	271	235	0.03%	0.004%
86	10.516	2942	2947	2950	rBV	155	206	0.02%	0.003%
87	10.577	2963	2966	2971	rVB4	765	695	0.08%	0.011%
88	10.616	2976	2978	2980	rBV	231	115	0.01%	0.002%
89	10.686	2997	3000	3002	rBV	310	202	0.02%	0.003%
90	10.754	3019	3021	3023	rBB	380	159	0.02%	0.002%
91	10.767	3023	3025	3026	rBV	244	102	0.01%	0.002%
92	10.918	3066	3072	3079	rVB5	1572	1924	0.23%	0.029%
93	10.950	3080	3082	3085	rBB	222	141	0.02%	0.002%
94	10.989	3086	3094	3095	rBV	169	263	0.03%	0.004%
95	11.198	3155	3159	3161	rBV	183	152	0.02%	0.002%
96	11.249	3163	3175	3194	rBV	413969	637384	76.63%	9.757%
97	11.622	3279	3291	3309	rBV	430699	680252	81.78%	10.413%
98	11.837	3355	3358	3362	rBV	220	235	0.03%	0.004%
99	11.879	3368	3371	3374	rBV	171	168	0.02%	0.003%
100	12.191	3465	3468	3469	rBV	290	160	0.02%	0.002%




Sum of corrected areas: 6532536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
Data File : VV024293.D
Acq On : 06 Jan 2022 14:14
Operator : SY/MD
Sample : N1009-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

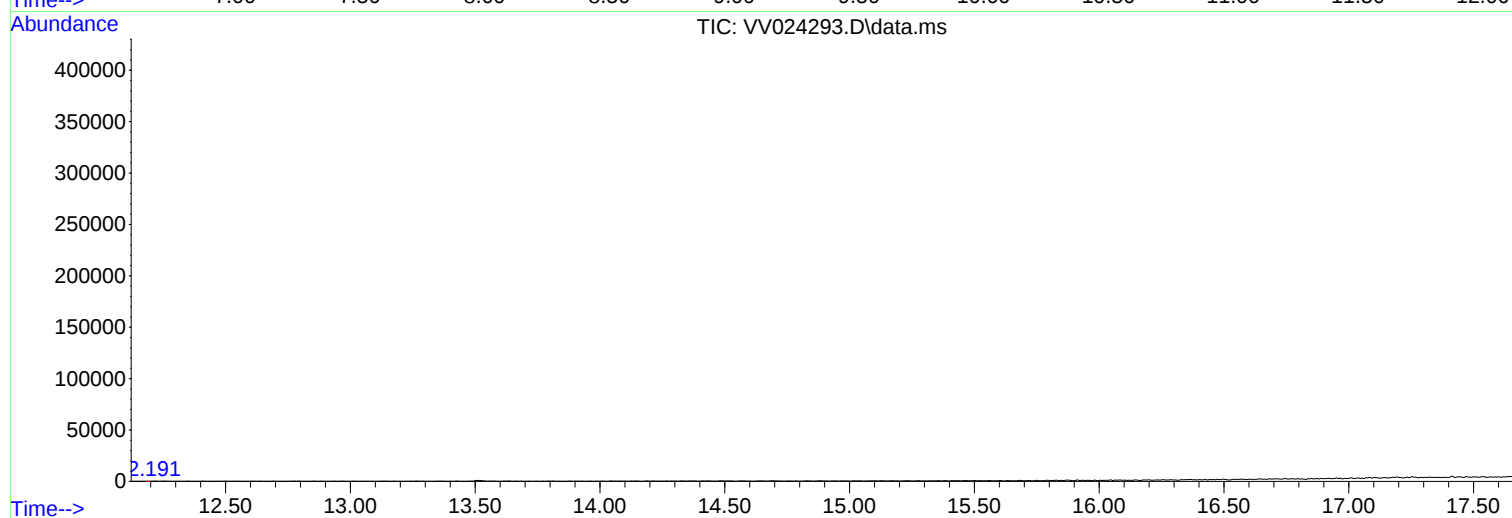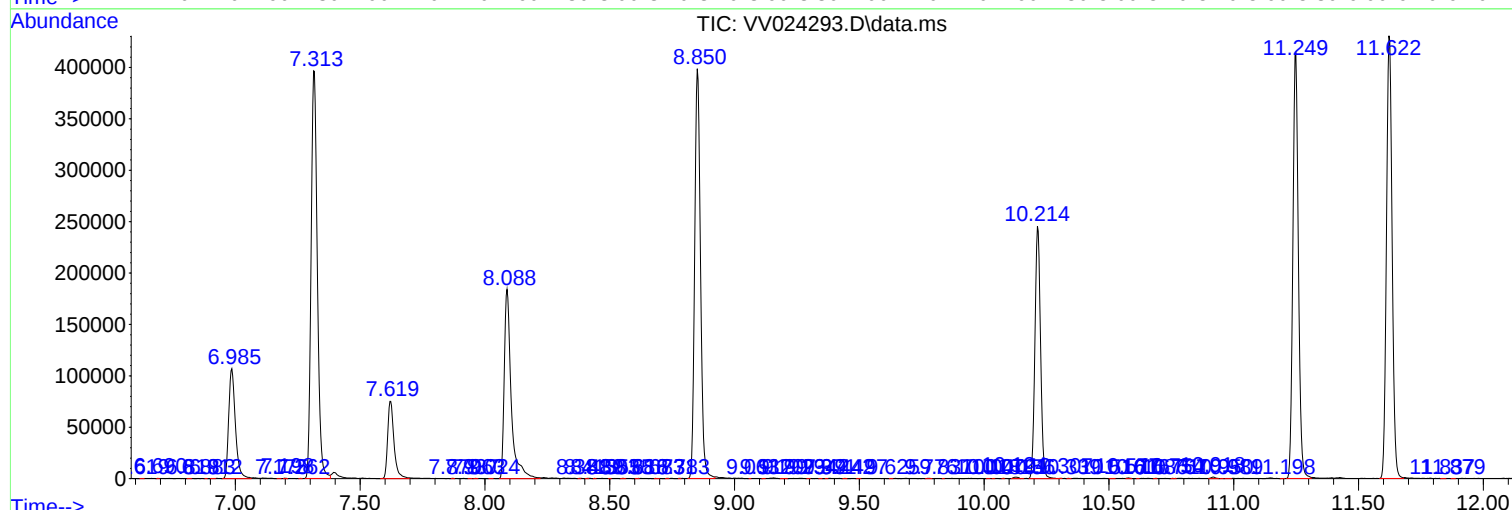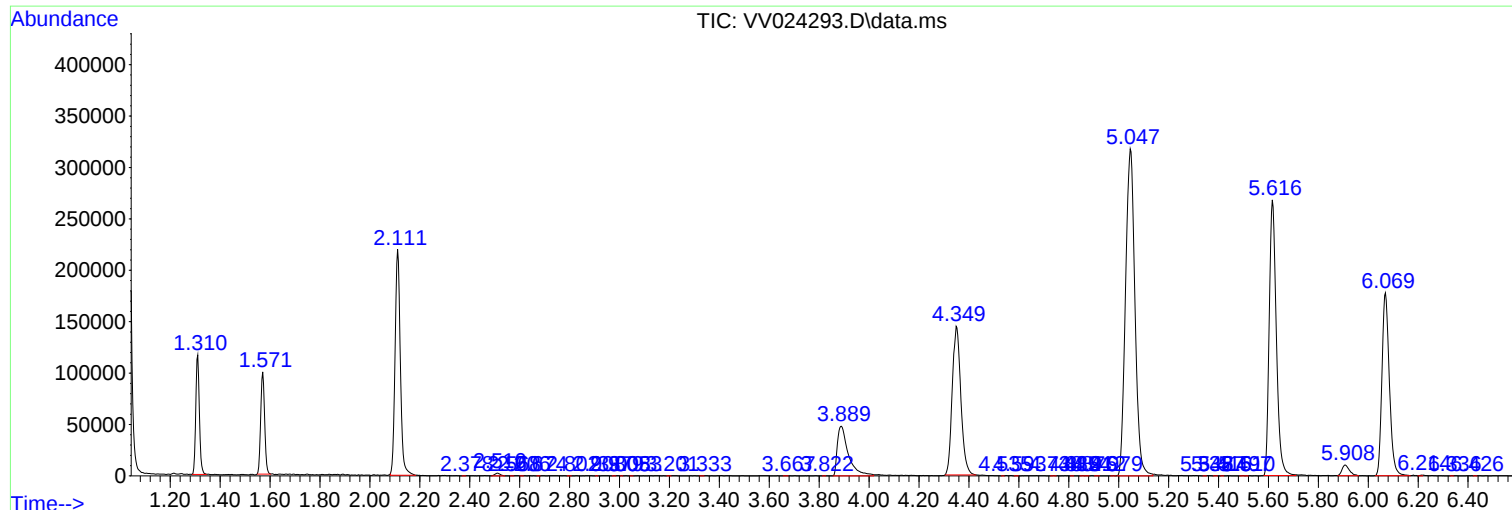

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
Data File : VV024293.D
Acq On : 06 Jan 2022 14:14
Operator : SY/MD
Sample : N1009-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
Data File : VV024293.D
Acq On : 06 Jan 2022 14:14
Operator : SY/MD
Sample : N1009-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc