


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010622\
 Data File : VV024285.D
 Acq On : 06 Jan 2022 10:06
 Operator : SY/MD
 Sample : BFB252
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB252

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 07 01:34:41 2022

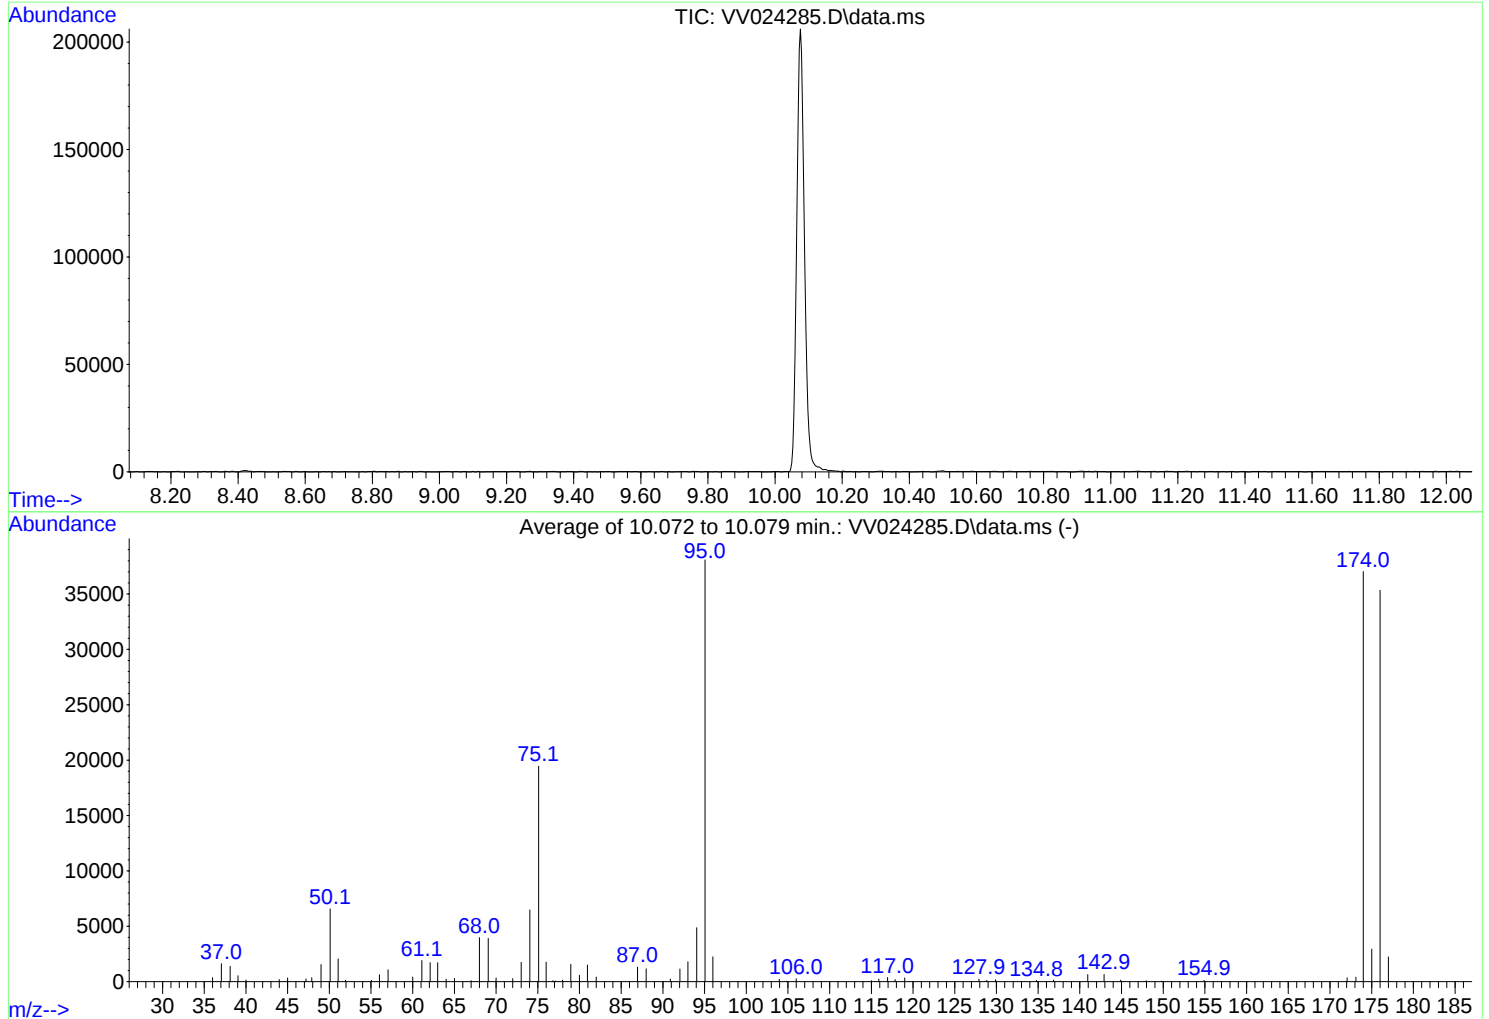

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	6568	PASS
75	95	30	80	51.1	19453	PASS
95	95	100	100	100.0	38085	PASS
96	95	5	9	5.9	2239	PASS
173	174	0.00	2	1.1	406	PASS
174	95	50	120	97.2	37035	PASS
175	174	5	9	7.9	2930	PASS
176	174	95	105	95.4	35336	PASS
177	176	5	10	6.3	2230	PASS

m/z	Abundance
44.00	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252

m/z	Abundance
36.00	337.0
37.00	1487.0
38.10	1309.0
39.00	523.0
40.00	107.0
44.00	278.0
45.00	287.0
47.10	176.0
47.90	303.0
49.00	1498.0
50.10	6257.0
51.00	1890.0
52.00	146.0
53.00	103.0
55.10	127.0
56.00	659.0
57.00	994.0
60.00	377.0
61.10	1770.0
62.10	1677.0
63.00	1694.0
64.00	239.0
65.00	254.0
68.00	3912.0
69.00	3656.0
70.00	362.0
72.00	277.0
73.00	1779.0
74.10	6359.0
75.10	18792.0
76.00	1639.0
76.80	115.0
77.90	165.0
79.00	1546.0
80.00	502.0
81.00	1504.0
82.00	365.0
87.00	1304.0
88.00	1223.0
90.90	213.0
92.00	1145.0
93.00	1726.0
94.00	4808.0
95.10	37184.0
96.00	2183.0
104.00	221.0
106.00	259.0
115.90	231.0
116.90	339.0
117.90	154.0
119.10	377.0
127.90	203.0
128.80	116.0
129.90	157.0
134.80	113.0
136.90	126.0
141.00	621.0
142.90	603.0
145.00	164.0
149.80	134.0
154.90	127.0
172.00	348.0
173.10	596.0
174.00	36576.0
175.00	2934.0
176.00	35288.0
177.00	2205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252

m/z	Abundance
36.00	376.0
37.00	1680.0
38.10	1450.0
39.10	526.0
40.00	148.0
44.00	317.0
45.00	339.0
47.20	244.0
47.90	374.0
49.00	1565.0
50.10	6669.0
51.10	2146.0
52.00	140.0
55.00	116.0
56.00	642.0
57.10	1095.0
60.00	435.0
61.10	1976.0
62.10	1764.0
63.00	1797.0
64.00	241.0
65.00	288.0
67.00	111.0
68.00	4129.0
69.10	4074.0
70.00	343.0
72.00	280.0
73.00	1850.0
74.10	6595.0
75.10	20064.0
76.00	1836.0
76.80	147.0
77.90	128.0
79.00	1599.0
80.00	615.0
81.00	1511.0
82.00	464.0
86.90	1321.0
88.00	1173.0
90.90	249.0
92.10	1157.0
93.00	1872.0
94.00	4990.0
95.10	39592.0
96.00	2295.0
104.00	238.0
106.00	284.0
115.00	121.0
115.90	257.0
117.00	390.0
117.90	176.0
119.00	326.0
127.90	257.0
128.80	127.0
129.90	191.0
134.80	121.0
136.80	151.0
140.90	646.0
142.90	661.0
144.90	137.0
147.90	129.0
154.90	127.0
172.10	360.0
173.10	622.0
174.00	38344.0
175.00	3029.0
176.00	36360.0
177.00	2297.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252

m/z	Abundance
36.00	377.0
37.10	1692.0
38.10	1382.0
39.00	543.0
40.00	179.0
44.00	365.0
45.00	353.0
47.20	309.0
47.90	360.0
49.00	1574.0
50.10	6777.0
51.10	2109.0
51.90	115.0
55.00	126.0
56.00	556.0
57.00	1103.0
60.00	429.0
61.10	1986.0
62.10	1726.0
63.00	1627.0
64.00	209.0
65.00	316.0
67.00	141.0
68.00	3873.0
69.10	3978.0
70.00	311.0
72.00	262.0
73.00	1623.0
74.00	6454.0
75.10	19504.0
76.00	1832.0
77.10	192.0
78.10	100.0
78.90	1538.0
80.00	634.0
80.90	1482.0
82.00	451.0
86.90	1299.0
88.00	1077.0
90.90	249.0
92.10	1110.0
93.00	1793.0
94.10	4809.0
95.00	37480.0
96.00	2239.0
103.90	206.0
104.80	119.0
106.00	256.0
115.00	120.0
115.90	224.0
117.00	391.0
117.80	218.0
118.90	299.0
127.90	257.0
128.90	111.0
129.90	172.0
134.80	109.0
136.80	151.0
140.90	625.0
142.90	701.0
144.80	125.0
148.00	155.0
154.90	115.0
172.10	358.0
174.00	36184.0
175.00	2826.0
176.00	34360.0
177.00	2189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252