

Data File : VV009187.D
Acq On : 07 Jan 2019 17:23
Operator : SY/MD
Sample : K1050-10
Misc : 6.39G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE9W7

Quant Time: Jan 08 00:31:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM010419S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 08 00:28:03 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	217162	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	203458	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	98922	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	29845	20.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.40%
7) Chloroethane-d5	1.58	69	32115	22.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.16%
10) 1,1-Dichloroethene-d2	2.13	63	75026	15.11	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.44%
20) 2-Butanone-d5	3.96	46	29913	28.63	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	57.26%
24) Chloroform-d	4.40	84	106815	23.36	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.44%
26) 1,2-Dichloroethane-d4	5.08	65	58452	23.90	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.60%
29) Benzene-d6	5.10	84	211474	23.33	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.32%
33) 1,2-Dichloropropane-d6	6.12	67	64203	24.70	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.80%
37) Toluene-d8	7.36	98	190516	22.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.12%
38) trans-1,3-Dichloropropene-	7.67	79	25651	20.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.20%
39) 2-Hexanone-d5	8.14	63	20241	33.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.00%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	56883	19.91	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.64%
61) 1,2-Dichlorobenzene-d4	11.67	152	80477	24.07	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.28%

Target Compounds


					Qvalue
13) Acetone	2.21	43	13080	8.832 ug/L	99
16) Methylene chloride	2.54	84	60284	18.581 ug/L	96
35) Trichloroethene	5.96	95	1954	0.620 ug/L	92
36) Methylcyclohexane	6.12	83	16412	3.117 ug/L #	19
40) 1,2-Dichloropropane	6.12	63	7088	2.689 ug/L #	85
44) Toluene	7.43	91	13873	1.176 ug/L	97
59) 1,2,3-Trichloropropane	11.30	75	10085	4.042 ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV009187.D
Acq On : 07 Jan 2019 17:23
Operator : SY/MD
Sample : K1050-10
Misc : 6.39G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE9W7

Quant Time: Jan 08 00:31:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM010419S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 08 00:28:03 2019
Response via : Initial Calibration

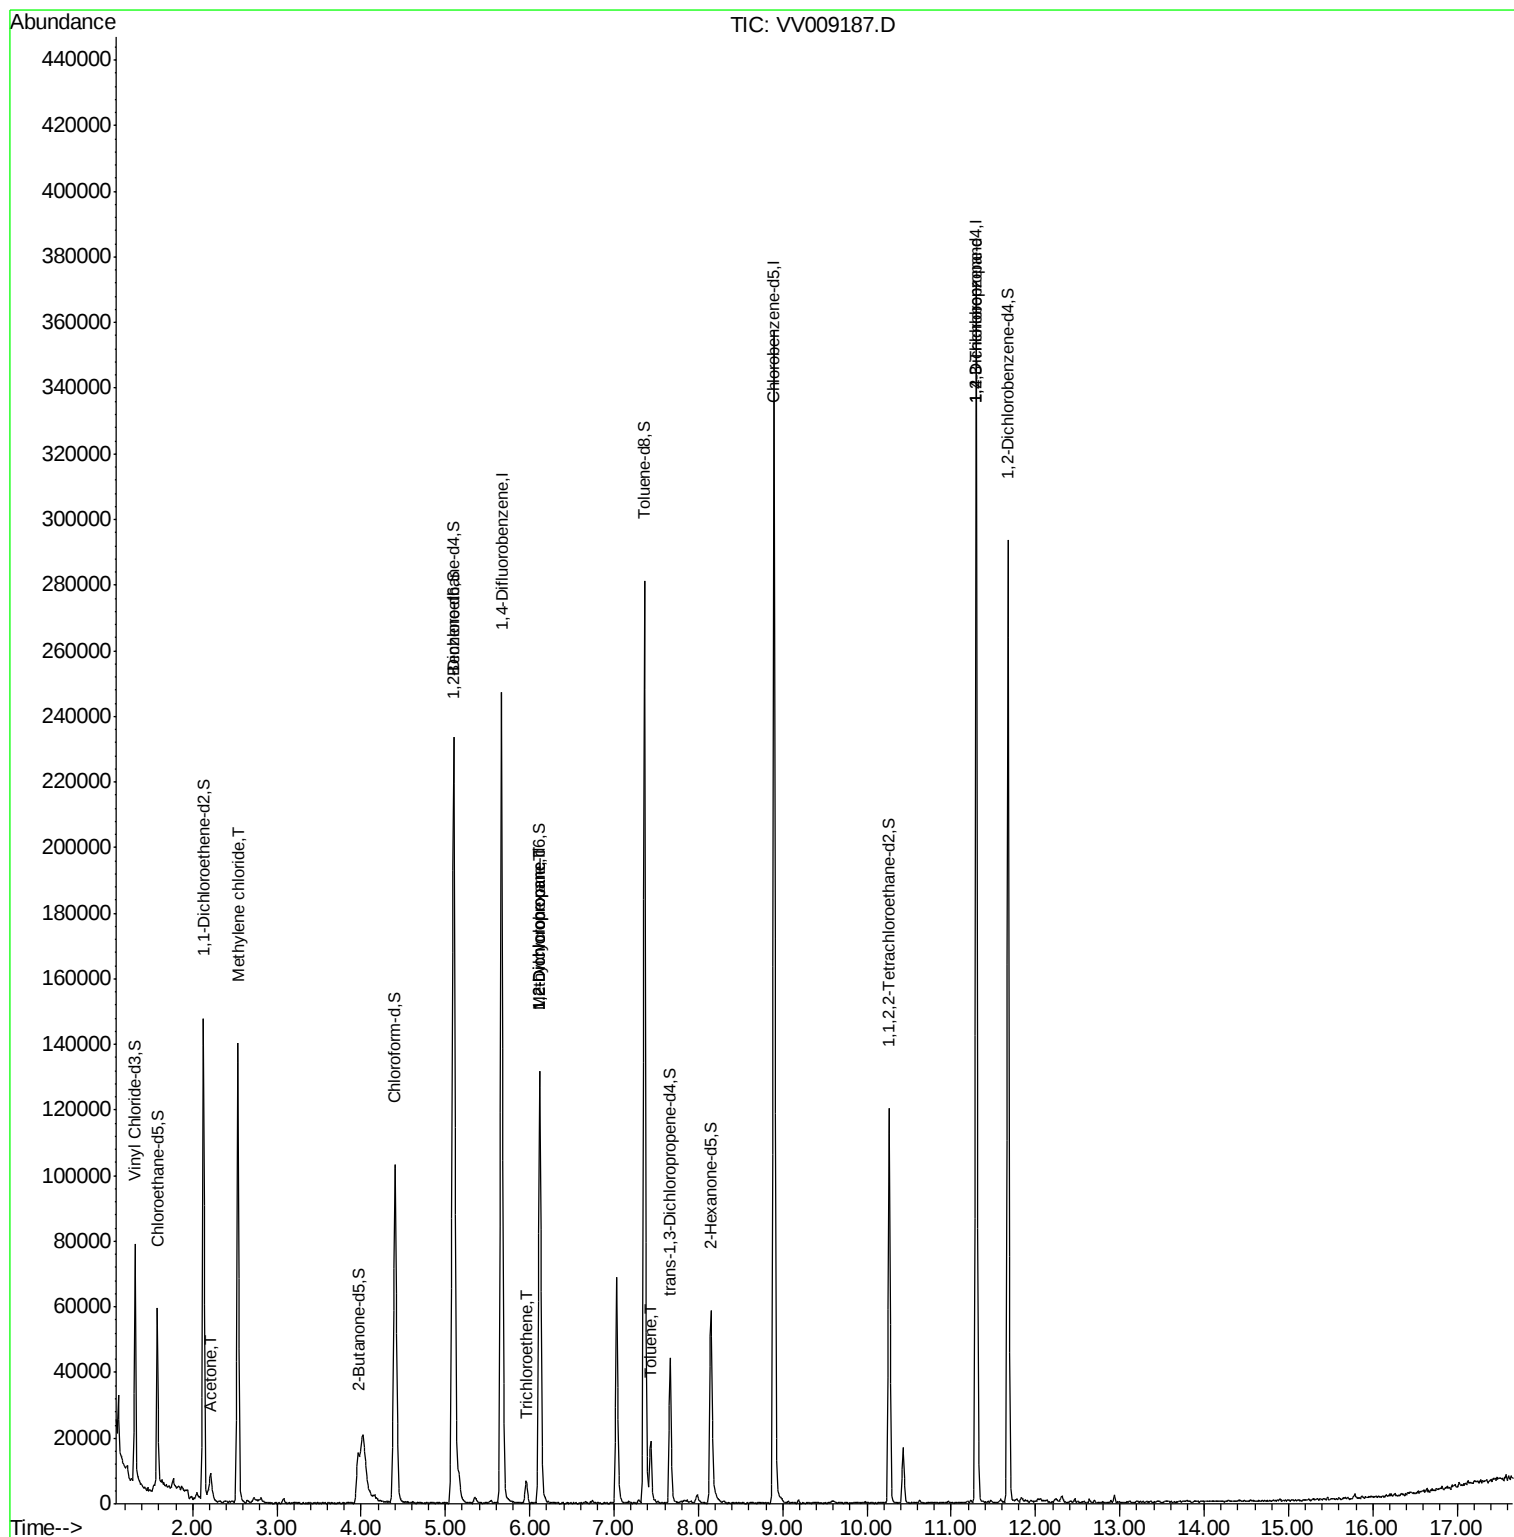

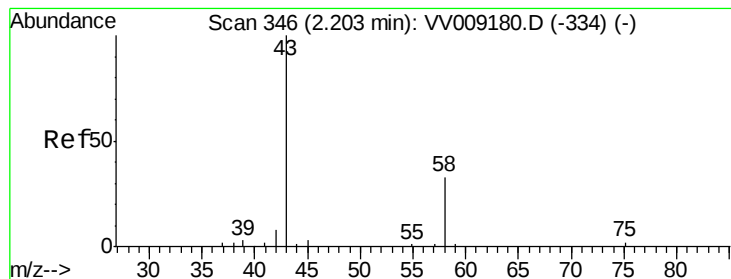

#13

Acetone

Concen: 8.832 ug/L

RT: 2.21 min Scan# 349

Delta R.T. 0.01 min

Lab File: VV009187.D

Acq: 07 Jan 2019 17:23

Instrument :

MSVOA_V

ClientSampleId :


BE9W7

Tgt Ion: 43 Resp: 13080

Ion Ratio Lower Upper




43 100

58 33.8 0.0 67.0

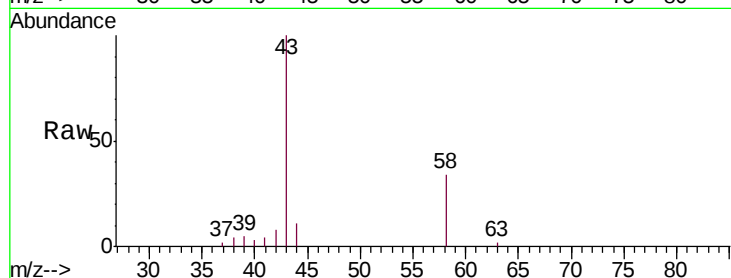

Abundance Ion 43.00 (42.70 to 43.70): VV009187.D (-349) (-)

Ion 58.00 (57.70 to 58.70): VV009187.D (-349) (-)

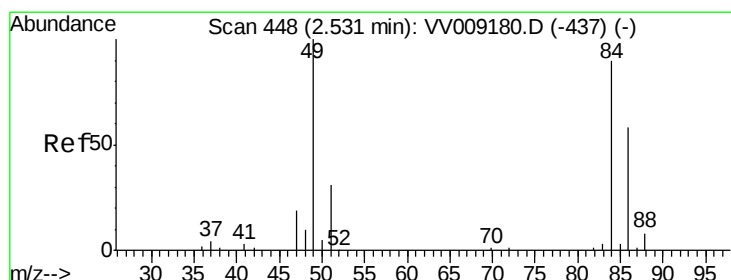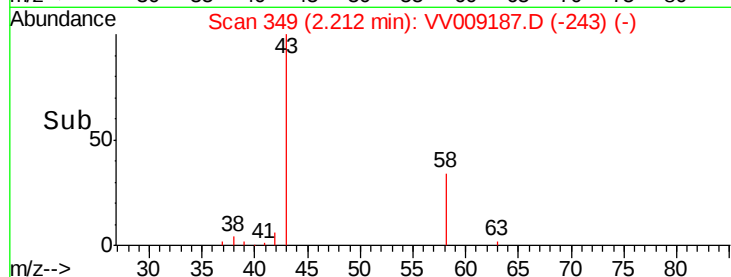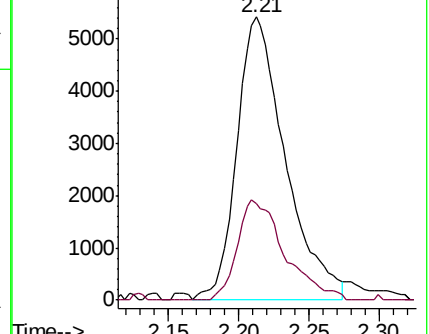

#16

Methylene chloride

Concen: 18.581 ug/L

RT: 2.54 min Scan# 450

Delta R.T. 0.01 min

Lab File: VV009187.D

Acq: 07 Jan 2019 17:23


Tgt Ion: 84 Resp: 60284

Ion Ratio Lower Upper

84 100

49 108.0 77.6 144.2



86 63.9 47.4 88.0

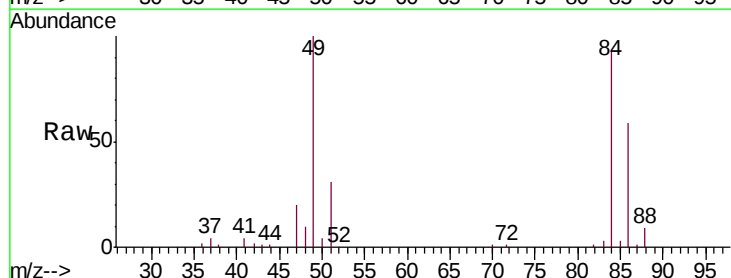


Abundance Ion 84.00 (83.70 to 84.70): VV009187.D (-450) (-)

Ion 49.00 (48.70 to 49.70): VV009187.D (-450) (-)

Ion 86.00 (85.70 to 86.70): VV009187.D (-450) (-)

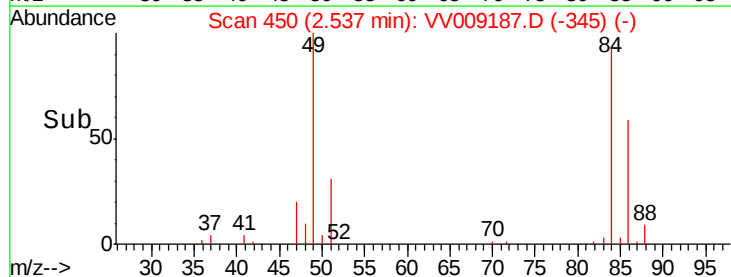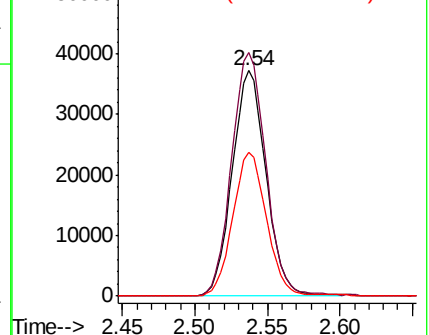

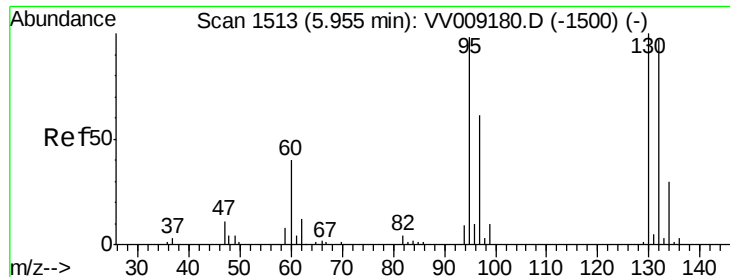

#35

Trichloroethene

Concen: 0.620 ug/L

RT: 5.96 min Scan# 1516

Delta R.T. 0.01 min

Lab File: VV009187.D

Acq: 07 Jan 2019 17:23

Instrument :

MSVOA_V

ClientSampleId :

BE9W7

Tgt Ion: 95 Resp: 1954


Ion Ratio Lower Upper

95 100

97 61.0 46.2 85.8

132 93.0 73.9 137.3

130 104.8 77.0 143.0



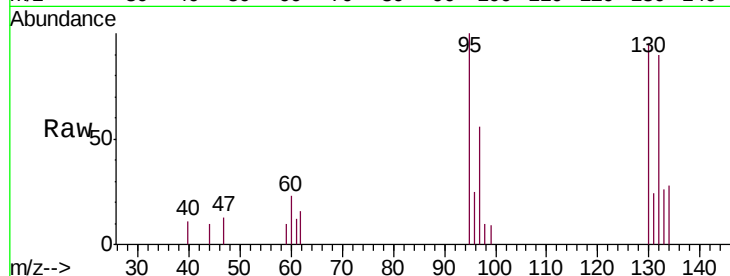


Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 97.00 (96.70 to 97.70): VV0

Ion 132.00 (131.70 to 132.70): VV0

Ion 130.00 (129.70 to 130.70): VV0

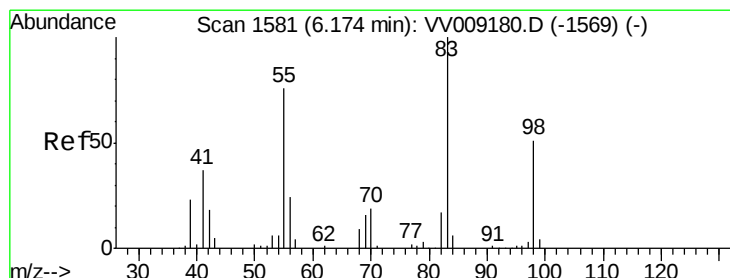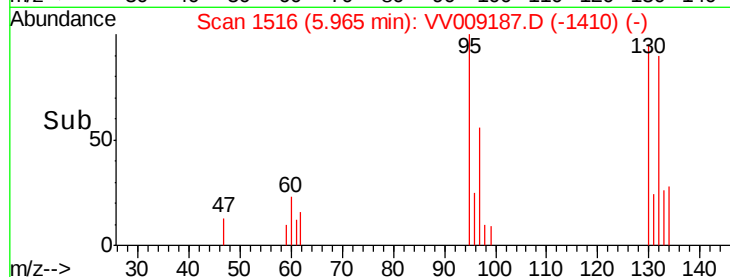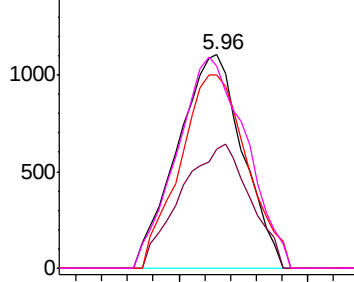

#36

Methylcyclohexane

Concen: 3.117 ug/L

RT: 6.12 min Scan# 1564

Delta R.T. -0.05 min

Lab File: VV009187.D

Acq: 07 Jan 2019 17:23


Tgt Ion: 83 Resp: 16412

Ion Ratio Lower Upper

83 100

55 0.4 58.5 87.7#



98 1.0 41.4 62.0#

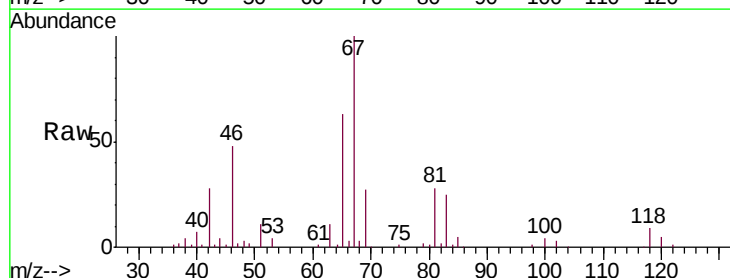


Abundance Ion 83.00 (82.70 to 83.70): VV0

Ion 55.00 (54.70 to 55.70): VV0

Ion 98.00 (97.70 to 98.70): VV0



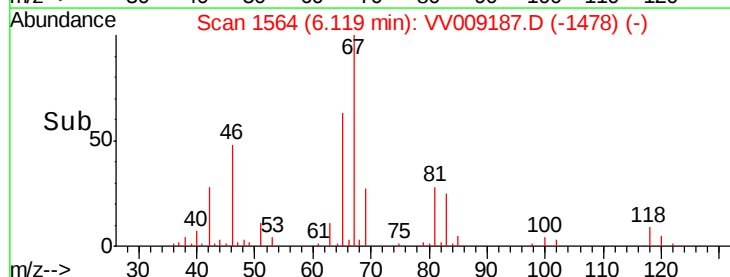
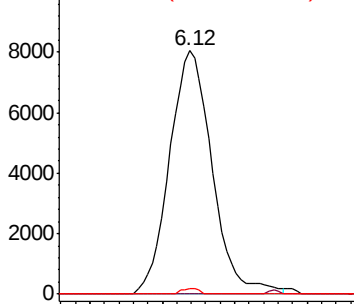


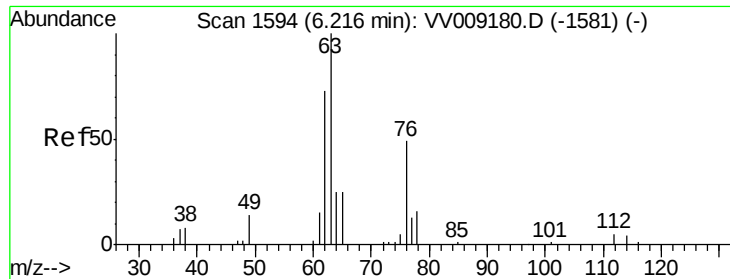

#40
 1,2-Dichloropropane
 Concen: 2.689 ug/L
 RT: 6.12 min Scan# 1564
 Delta R.T. -0.10 min
 Lab File: VV009187.D
 Acq: 07 Jan 2019 17:23




Instrument :
 MSVOA_V
 ClientSampleId :
 BE9W7


Tgt Ion: 63 Resp: 7088
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.9 5.9#

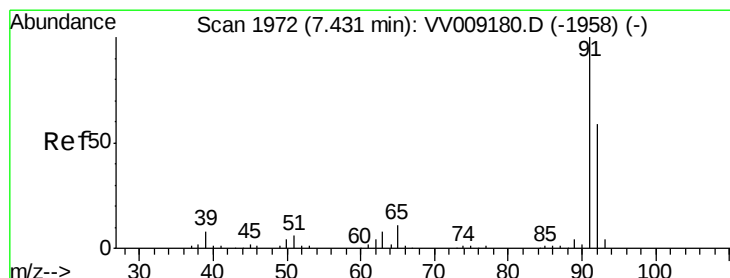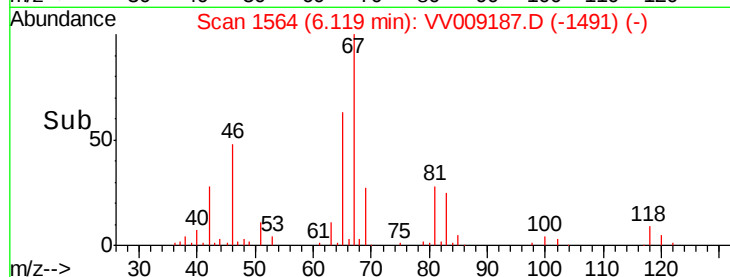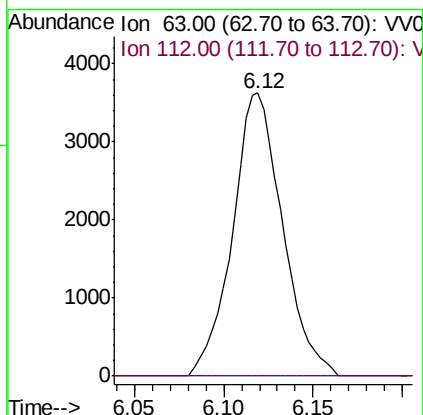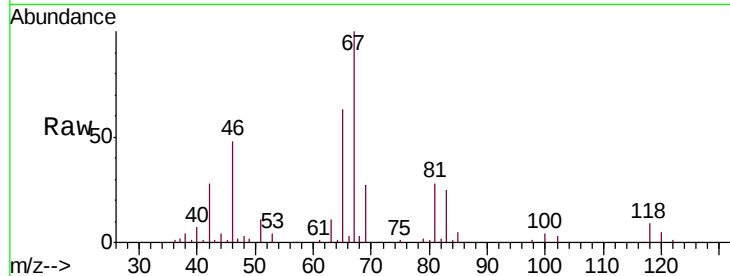

#44
 Toluene
 Concen: 1.176 ug/L
 RT: 7.43 min Scan# 1973
 Delta R.T. 0.00 min
 Lab File: VV009187.D
 Acq: 07 Jan 2019 17:23

Tgt Ion: 91 Resp: 13873
 Ion Ratio Lower Upper
 91 100
 92 57.5 41.7 77.5

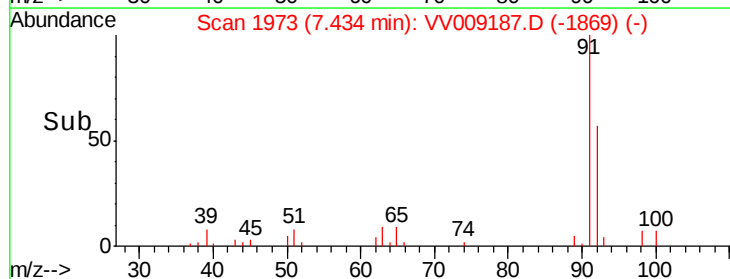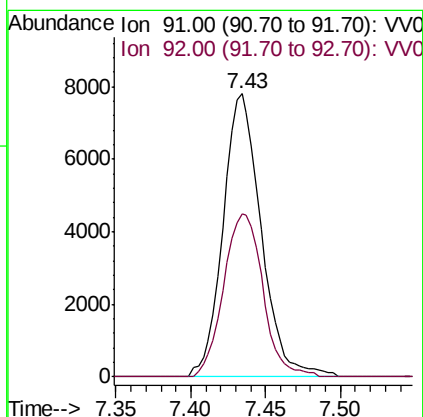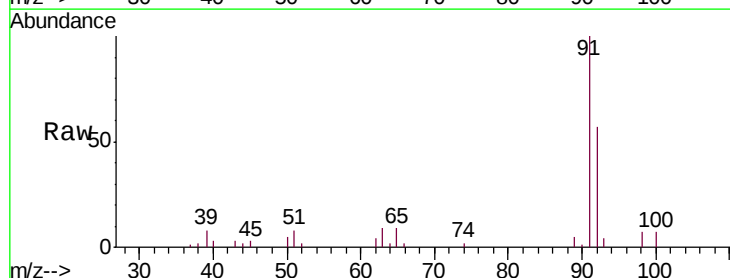

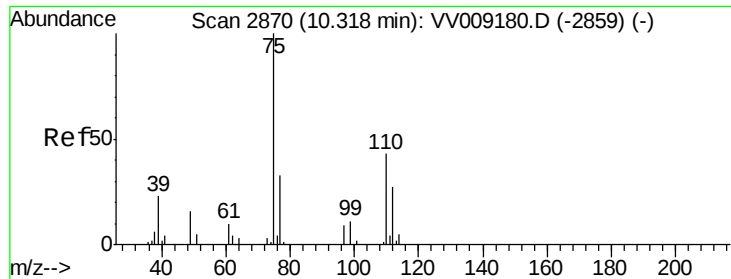

#59

1,2,3-Trichloropropane

Concen: 4.042 ug/L

RT: 11.30 min Scan# 3174

Delta R.T. 0.98 min

Lab File: VV009187.D

Acq: 07 Jan 2019 17:23

Instrument :

MSVOA_V

ClientSampleId :

BE9W7

Tgt Ion: 75 Resp: 10085

Ion Ratio Lower Upper

75 100

77 38.1 25.0 37.6#

