


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010719\
Data File : VV009179.D
Acq On : 07 Jan 2019 09:32
Operator : SY/MD
Sample : BFB69
Misc : 5.00 G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB69

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM010419S.M
Title : VOC Analysis
Last Update : Tue Jan 08 00:28:03 2019

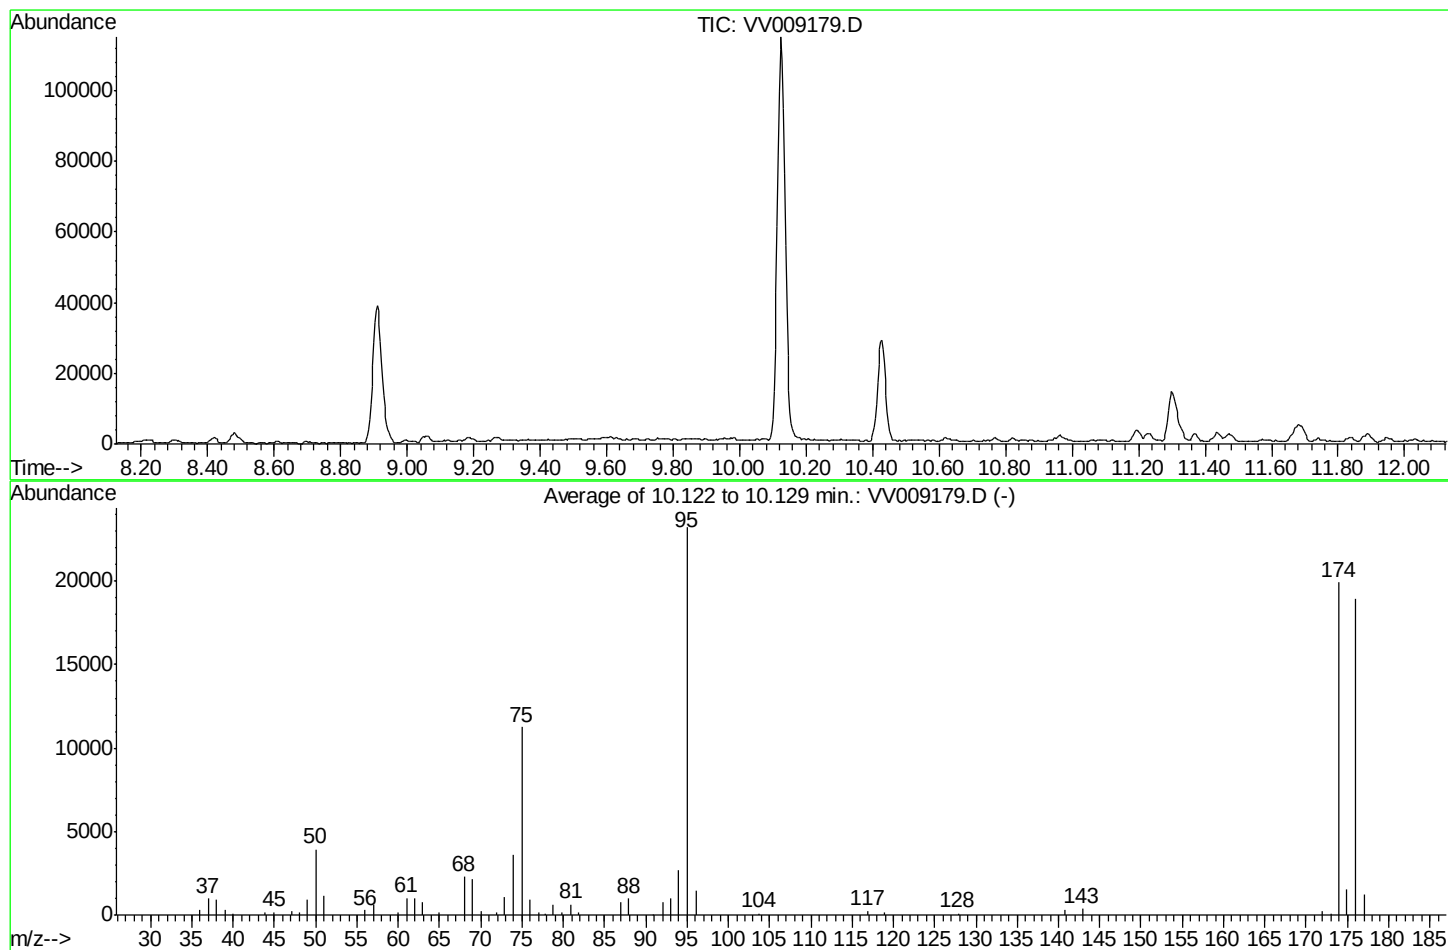

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	3915	PASS
75	95	30	80	48.4	11252	PASS
95	95	100	100	100.0	23224	PASS
96	95	5	9	6.4	1490	PASS
173	174	0.00	2	0.4	79	PASS
174	95	50	120	85.8	19925	PASS
175	174	5	9	7.8	1547	PASS
176	174	95	101	95.1	18952	PASS
177	176	5	9	6.5	1225	PASS

Scan 2797 (10.084 min): VV009179.D
BFB69

m/z	Abundance
35.90	632.0
37.90	214.0
43.80	167.0
54.90	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	952.0
37.00	928.0
38.00	1089.0
39.00	322.0
43.90	333.0
45.00	145.0
47.00	274.0
48.00	149.0
48.90	988.0
50.00	3978.0
51.00	1222.0
56.00	277.0
57.00	617.0
59.90	200.0
61.00	990.0
61.90	1023.0
63.00	749.0
64.90	162.0
68.00	2239.0
69.00	2086.0
70.00	212.0
71.90	149.0
72.90	1073.0
74.00	3596.0
75.00	11181.0
76.00	1023.0
77.00	183.0
77.80	135.0
78.80	590.0
79.80	157.0
81.00	634.0
81.90	169.0
86.90	687.0
88.00	972.0
90.90	107.0
92.00	703.0
93.00	959.0
94.00	2559.0
95.00	23632.0
96.00	1471.0
103.80	106.0
116.90	304.0
118.90	128.0
140.80	260.0
143.00	317.0
171.90	220.0
174.00	19712.0
175.00	1499.0
176.00	19072.0
177.00	1259.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
35.00	943.0
37.00	1031.0
38.00	1149.0
39.00	287.0
40.00	114.0
44.00	313.0
45.00	157.0
47.10	278.0
48.00	152.0
48.90	918.0
50.00	4016.0
51.00	1145.0
56.00	316.0
57.00	604.0
59.90	187.0
61.00	1098.0
61.90	986.0
63.00	791.0
64.90	145.0
68.00	2384.0
69.00	2137.0
70.00	204.0
71.90	155.0
72.90	1124.0
74.00	3768.0
75.00	11572.0
76.00	980.0
77.00	183.0
77.90	108.0
78.80	599.0
79.90	160.0
81.00	640.0
81.90	173.0
86.90	803.0
88.00	1011.0
92.00	760.0
93.00	998.0
94.00	2803.0
95.00	23824.0
96.10	1536.0
103.80	118.0
116.90	271.0
118.80	148.0
127.90	124.0
140.80	306.0
142.90	369.0
172.00	262.0
173.00	239.0
174.00	20488.0
175.00	1593.0
176.00	19504.0
177.00	1256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
35.00	855.0
37.00	1012.0
38.00	1183.0
39.00	250.0
40.00	139.0
44.00	290.0
45.00	183.0
47.20	237.0
48.00	109.0
48.90	811.0
50.00	3752.0
51.00	1010.0
56.00	319.0
57.00	598.0
60.00	171.0
61.00	1011.0
62.00	940.0
62.90	794.0
65.00	123.0
68.00	2278.0
69.00	2168.0
70.00	174.0
72.00	155.0
72.90	1076.0
74.00	3535.0
75.00	11005.0
76.00	852.0
77.00	135.0
78.80	558.0
79.90	168.0
80.90	569.0
81.90	150.0
86.90	917.0
87.90	959.0
92.00	778.0
93.00	938.0
94.00	2783.0
95.00	22216.0
96.10	1464.0
103.70	107.0
116.80	178.0
118.80	179.0
127.90	121.0
140.80	291.0
142.90	377.0
172.00	278.0
174.00	19576.0
174.90	1551.0
176.00	18280.0
177.00	1162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69