

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019915.D
 Acq On : 07 Jan 2021 12:15
 Operator : SY/MD
 Sample : M1017-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.306	61	67	81	rVB	208026	213501	0.96%	0.575%
2	1.569	142	149	160	rVB	197627	216317	0.97%	0.583%
3	2.110	308	317	339	rVB	380312	601767	2.70%	1.622%
4	2.772	512	523	535	rBV4	8119	17565	0.08%	0.047%
5	2.984	587	589	593	rVB4	865	366	0.00%	0.001%
6	3.081	616	619	621	rVB3	717	331	0.00%	0.001%
7	3.093	621	623	629	rVB5	1000	788	0.00%	0.002%
8	3.122	629	632	633	rBV2	548	282	0.00%	0.001%
9	3.280	677	681	685	rBV4	1262	1053	0.00%	0.003%
10	3.344	698	701	705	rBV3	827	699	0.00%	0.002%
11	3.380	710	712	713	rVB	253	84	0.00%	0.000%
12	3.402	713	719	722	rBV4	1056	1074	0.00%	0.003%
13	3.444	728	732	733	rBV2	735	469	0.00%	0.001%
14	3.470	739	740	741	rBV	460	148	0.00%	0.000%
15	3.540	760	762	766	rVB3	429	257	0.00%	0.001%
16	3.560	766	768	770	rBV3	833	378	0.00%	0.001%
17	3.579	770	774	776	rBV4	976	681	0.00%	0.002%
18	3.624	785	788	790	rVB3	733	438	0.00%	0.001%
19	3.643	790	794	796	rBV4	923	672	0.00%	0.002%
20	3.695	803	810	817	rBV5	1287	1953	0.01%	0.005%
21	3.753	823	828	830	rBV3	1092	1023	0.00%	0.003%
22	3.817	846	848	851	rBV3	775	454	0.00%	0.001%
23	3.849	856	858	859	rBV	669	365	0.00%	0.001%
24	3.888	859	870	909	rBV	162425	488902	2.20%	1.318%
25	4.351	1000	1014	1042	rVB	294553	721553	3.24%	1.945%
26	4.643	1102	1105	1107	rBV2	798	414	0.00%	0.001%
27	4.714	1125	1127	1131	rBV4	961	761	0.00%	0.002%
28	4.743	1134	1136	1141	rVB3	1120	697	0.00%	0.002%
29	4.775	1141	1146	1147	rBV4	990	870	0.00%	0.002%
30	4.871	1174	1176	1178	rBV3	673	313	0.00%	0.001%
31	4.936	1194	1196	1201	rBV6	644	423	0.00%	0.001%
32	4.978	1207	1209	1213	rVB4	1154	865	0.00%	0.002%
33	5.048	1213	1231	1267	rBV2	667384	1767227	7.93%	4.763%
34	5.621	1397	1409	1431	rBV	612184	1213449	5.45%	3.271%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019915.D
 Acq On : 07 Jan 2021 12:15
 Operator : SY/MD
 Sample : M1017-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	5.920	1488	1502	1525	rBV2	281835	592730	2.66%	1.598%
36	6.074	1537	1550	1571	rBV	410465	833949	3.74%	2.248%
37	6.338	1627	1632	1634	rBV5	1414	1338	0.01%	0.004%
38	6.550	1695	1698	1701	rBV4	1106	791	0.00%	0.002%
39	6.585	1708	1709	1712	rBV2	557	285	0.00%	0.001%
40	6.855	1792	1793	1797	rBV4	436	249	0.00%	0.001%
41	6.933	1815	1817	1820	rBV2	426	251	0.00%	0.001%
42	6.990	1823	1835	1855	rVV	211534	384192	1.72%	1.036%
43	7.322	1925	1938	1960	rBV	725871	1283237	5.76%	3.459%
44	7.624	2023	2032	2052	rBV	145158	253704	1.14%	0.684%
45	7.887	2111	2114	2115	rBV3	585	357	0.00%	0.001%
46	7.981	2128	2143	2167	rBV	13577942	22272795	100.00%	60.035%
47	8.093	2169	2178	2215	rVB2	504972	973431	4.37%	2.624%
48	8.855	2404	2415	2440	rBV	927159	1522014	6.83%	4.103%
49	9.122	2496	2498	2502	rBV2	1546	870	0.00%	0.002%
50	9.225	2528	2530	2533	rVB3	838	403	0.00%	0.001%
51	9.347	2566	2568	2572	rBV3	718	473	0.00%	0.001%
52	9.383	2578	2579	2581	rBV	568	185	0.00%	0.000%
53	9.463	2601	2604	2605	rBV2	579	296	0.00%	0.001%
54	9.601	2645	2647	2651	rVB3	1268	689	0.00%	0.002%
55	9.804	2707	2710	2712	rBV3	730	514	0.00%	0.001%
56	10.032	2777	2781	2784	rBV2	912	860	0.00%	0.002%
57	10.132	2810	2812	2816	rVB5	1109	530	0.00%	0.001%
58	10.151	2816	2818	2825	rVB6	879	951	0.00%	0.003%
59	10.222	2825	2840	2860	rBV	564075	888937	3.99%	2.396%
60	10.305	2863	2866	2870	rBV5	932	842	0.00%	0.002%
61	10.547	2937	2941	2947	rBV6	1574	1834	0.01%	0.005%
62	10.630	2963	2967	2971	rBV5	1017	1098	0.00%	0.003%
63	10.714	2991	2993	2999	rVB4	1293	885	0.00%	0.002%
64	10.739	2999	3001	3002	rBV2	656	265	0.00%	0.001%
65	10.749	3002	3004	3006	rVB	671	231	0.00%	0.001%
66	10.846	3031	3034	3038	rBV3	636	518	0.00%	0.001%
67	11.048	3093	3097	3098	rBV2	768	544	0.00%	0.001%
68	11.096	3109	3112	3114	rBV3	1014	636	0.00%	0.002%
69	11.128	3118	3122	3125	rVB2	916	787	0.00%	0.002%
70	11.254	3149	3161	3184	rBV	942710	1480740	6.65%	3.991%
71	11.479	3229	3231	3232	rBV2	1282	541	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019915.D
 Acq On : 07 Jan 2021 12:15
 Operator : SY/MD
 Sample : M1017-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	11.630	3266	3278	3298	rBV	856240	1332640	5.98%	3.592%
73	11.868	3350	3352	3354	rBV2	740	302	0.00%	0.001%
74	11.993	3389	3391	3393	rBV2	566	244	0.00%	0.001%
75	12.251	3468	3471	3474	rBV4	1082	895	0.00%	0.002%
76	12.476	3538	3541	3543	rVB2	745	387	0.00%	0.001%
77	13.016	3705	3709	3711	rBV3	1294	1037	0.00%	0.003%
78	13.058	3719	3722	3725	rBV4	910	625	0.00%	0.002%
79	13.122	3739	3742	3747	rBV5	988	990	0.00%	0.003%
80	13.222	3769	3773	3775	rBV2	1085	852	0.00%	0.002%
81	13.842	3960	3966	3971	rBV5	1129	1360	0.01%	0.004%
82	14.569	4188	4192	4194	rBV4	1229	1022	0.00%	0.003%


Sum of corrected areas: 37099445

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010721\
Data File : VV019915.D
Acq On : 07 Jan 2021 12:15
Operator : SY/MD
Sample : M1017-06 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

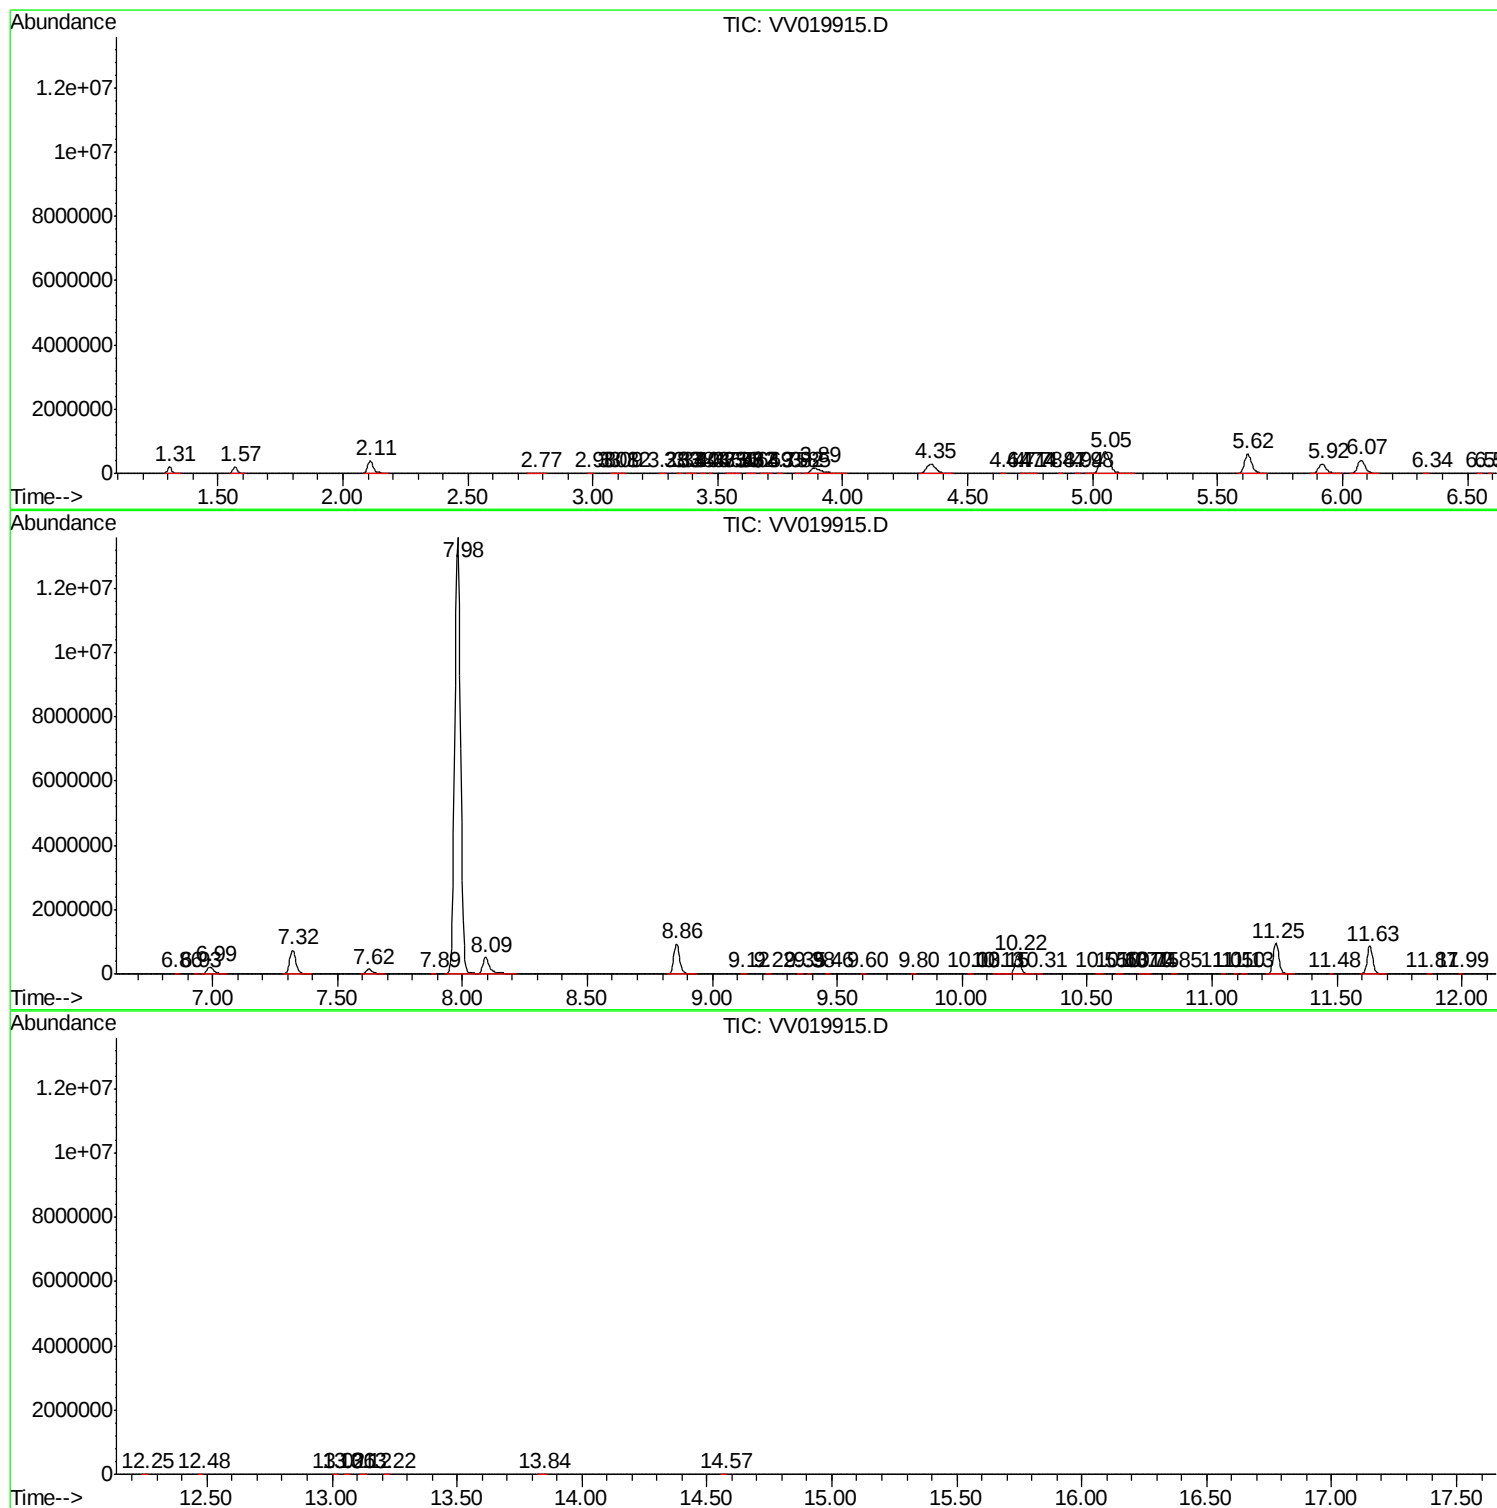

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010721\
Data File : VV019915.D
Acq On : 07 Jan 2021 12:15
Operator : SY/MD
Sample : M1017-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV010721\
Data File : VV019915.D
Acq On : 07 Jan 2021 12:15
Operator : SY/MD
Sample : M1017-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc