

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019918.D
 Acq On : 07 Jan 2021 13:35
 Operator : SY/MD
 Sample : M1016-10 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	79	rVB	213395	209383	11.85%	1.436%
2	1.570	142	149	159	rVB	195085	219783	12.44%	1.508%
3	2.110	308	317	351	rVB	383766	608001	34.40%	4.171%
4	2.611	465	473	475	rBV7	1671	1693	0.10%	0.012%
5	2.672	489	492	494	rBV3	1514	807	0.05%	0.006%
6	2.750	513	516	517	rBV3	723	411	0.02%	0.003%
7	2.785	525	527	530	rBV4	725	297	0.02%	0.002%
8	2.869	551	553	556	rVB3	644	255	0.01%	0.002%
9	3.026	600	602	605	rBV3	731	395	0.02%	0.003%
10	3.126	628	633	635	rBV4	689	574	0.03%	0.004%
11	3.187	649	652	654	rBV4	596	430	0.02%	0.003%
12	3.200	654	656	661	rVB3	824	563	0.03%	0.004%
13	3.264	674	676	679	rVB2	1288	752	0.04%	0.005%
14	3.287	679	683	686	rBV4	698	768	0.04%	0.005%
15	3.335	695	698	701	rVB5	1146	748	0.04%	0.005%
16	3.389	712	715	718	rVB4	758	491	0.03%	0.003%
17	3.405	718	720	721	rBV	535	266	0.02%	0.002%
18	3.463	734	738	742	rBV5	1301	1009	0.06%	0.007%
19	3.521	753	756	760	rVB3	774	646	0.04%	0.004%
20	3.547	760	764	768	rBV4	1058	878	0.05%	0.006%
21	3.576	770	773	774	rBV2	580	326	0.02%	0.002%
22	3.624	784	788	790	rBV2	537	328	0.02%	0.002%
23	3.695	804	810	811	rBV4	796	722	0.04%	0.005%
24	3.772	823	834	837	rBV8	1420	2353	0.13%	0.016%
25	3.820	844	849	850	rBV4	677	502	0.03%	0.003%
26	3.849	855	858	860	rBV2	795	610	0.03%	0.004%
27	3.894	860	872	911	rBV2	145795	475019	26.88%	3.259%
28	4.351	995	1014	1039	rBV	301807	746148	42.22%	5.119%
29	4.769	1140	1144	1147	rBV5	1670	1094	0.06%	0.008%
30	4.785	1147	1149	1150	rBV2	564	230	0.01%	0.002%
31	5.048	1214	1231	1266	rBV2	677904	1767259	100.00%	12.123%
32	5.409	1339	1343	1344	rBV2	1045	706	0.04%	0.005%
33	5.618	1394	1408	1435	rBV	641910	1293572	73.20%	8.874%
34	5.907	1490	1498	1514	rVB3	39190	77955	4.41%	0.535%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019918.D
 Acq On : 07 Jan 2021 13:35
 Operator : SY/MD
 Sample : M1016-10 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	6.071	1536	1549	1579	rBV	413696	850319	48.12%	5.833%
36	6.434	1660	1662	1666	rVB2	1036	668	0.04%	0.005%
37	6.450	1666	1667	1669	rBV2	374	142	0.01%	0.001%
38	6.463	1669	1671	1673	rBV3	441	295	0.02%	0.002%
39	6.476	1673	1675	1677	rVV	502	215	0.01%	0.001%
40	6.547	1693	1697	1700	rBV3	972	804	0.05%	0.006%
41	6.560	1700	1701	1703	rBV3	501	215	0.01%	0.001%
42	6.618	1716	1719	1720	rBV2	1407	564	0.03%	0.004%
43	6.743	1756	1758	1760	rBV3	738	363	0.02%	0.002%
44	6.872	1797	1798	1802	rVB2	1057	613	0.03%	0.004%
45	6.894	1802	1805	1808	rBV4	946	747	0.04%	0.005%
46	6.987	1823	1834	1860	rBV	208720	387529	21.93%	2.658%
47	7.319	1925	1937	1959	rBV	736887	1293596	73.20%	8.874%
48	7.624	2023	2032	2054	rBV	146343	254862	14.42%	1.748%
49	7.878	2109	2111	2113	rBV3	728	457	0.03%	0.003%
50	7.984	2136	2144	2157	rVB9	6234	12097	0.68%	0.083%
51	8.093	2168	2178	2216	rBV2	463631	954928	54.03%	6.551%
52	8.566	2323	2325	2328	rBV4	909	512	0.03%	0.004%
53	8.656	2351	2353	2355	rBV2	721	426	0.02%	0.003%
54	8.791	2390	2395	2397	rBV5	1085	973	0.06%	0.007%
55	8.855	2403	2415	2437	rBV	988955	1605904	90.87%	11.016%
56	9.482	2608	2610	2613	rBV2	777	588	0.03%	0.004%
57	9.630	2654	2656	2657	rBV	478	163	0.01%	0.001%
58	9.746	2689	2692	2695	rVB3	1466	791	0.04%	0.005%
59	10.106	2802	2804	2805	rBV	717	251	0.01%	0.002%
60	10.154	2818	2819	2822	rVB2	720	334	0.02%	0.002%
61	10.222	2828	2840	2861	rBV	546226	866809	49.05%	5.946%
62	10.331	2872	2874	2879	rVB4	1121	696	0.04%	0.005%
63	10.531	2933	2936	2937	rBV2	748	343	0.02%	0.002%
64	10.926	3057	3059	3067	rVB6	949	805	0.05%	0.006%
65	11.006	3082	3084	3088	rVB4	1189	807	0.05%	0.006%
66	11.026	3088	3090	3092	rBV3	699	482	0.03%	0.003%
67	11.151	3127	3129	3132	rVB4	838	420	0.02%	0.003%
68	11.177	3135	3137	3140	rVB3	1110	498	0.03%	0.003%
69	11.257	3149	3162	3192	rBV	1006103	1571499	88.92%	10.780%
70	11.630	3266	3278	3300	rBV	853901	1346149	76.17%	9.235%
71	12.016	3396	3398	3401	rBV3	834	535	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
Data File : VV019918.D
Acq On : 07 Jan 2021 13:35
Operator : SY/MD
Sample : M1016-10 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Title : VOC Analysis

72	12.090	3418	3421	3424	rBV3	834	600	0.03%	0.004%
73	12.486	3542	3544	3545	rBV	894	391	0.02%	0.003%
74	12.521	3552	3555	3557	rBV3	820	472	0.03%	0.003%
75	12.640	3590	3592	3596	rBV3	748	420	0.02%	0.003%
76	12.801	3640	3642	3645	rBV2	760	441	0.02%	0.003%
77	13.051	3718	3720	3725	rBV4	905	609	0.03%	0.004%
78	13.649	3903	3906	3910	rBV3	1357	1096	0.06%	0.008%
79	13.955	3999	4001	4004	rBV4	1312	900	0.05%	0.006%


Sum of corrected areas: 14577302

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010721\
Data File : VV019918.D
Acq On : 07 Jan 2021 13:35
Operator : SY/MD
Sample : M1016-10 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG4W8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

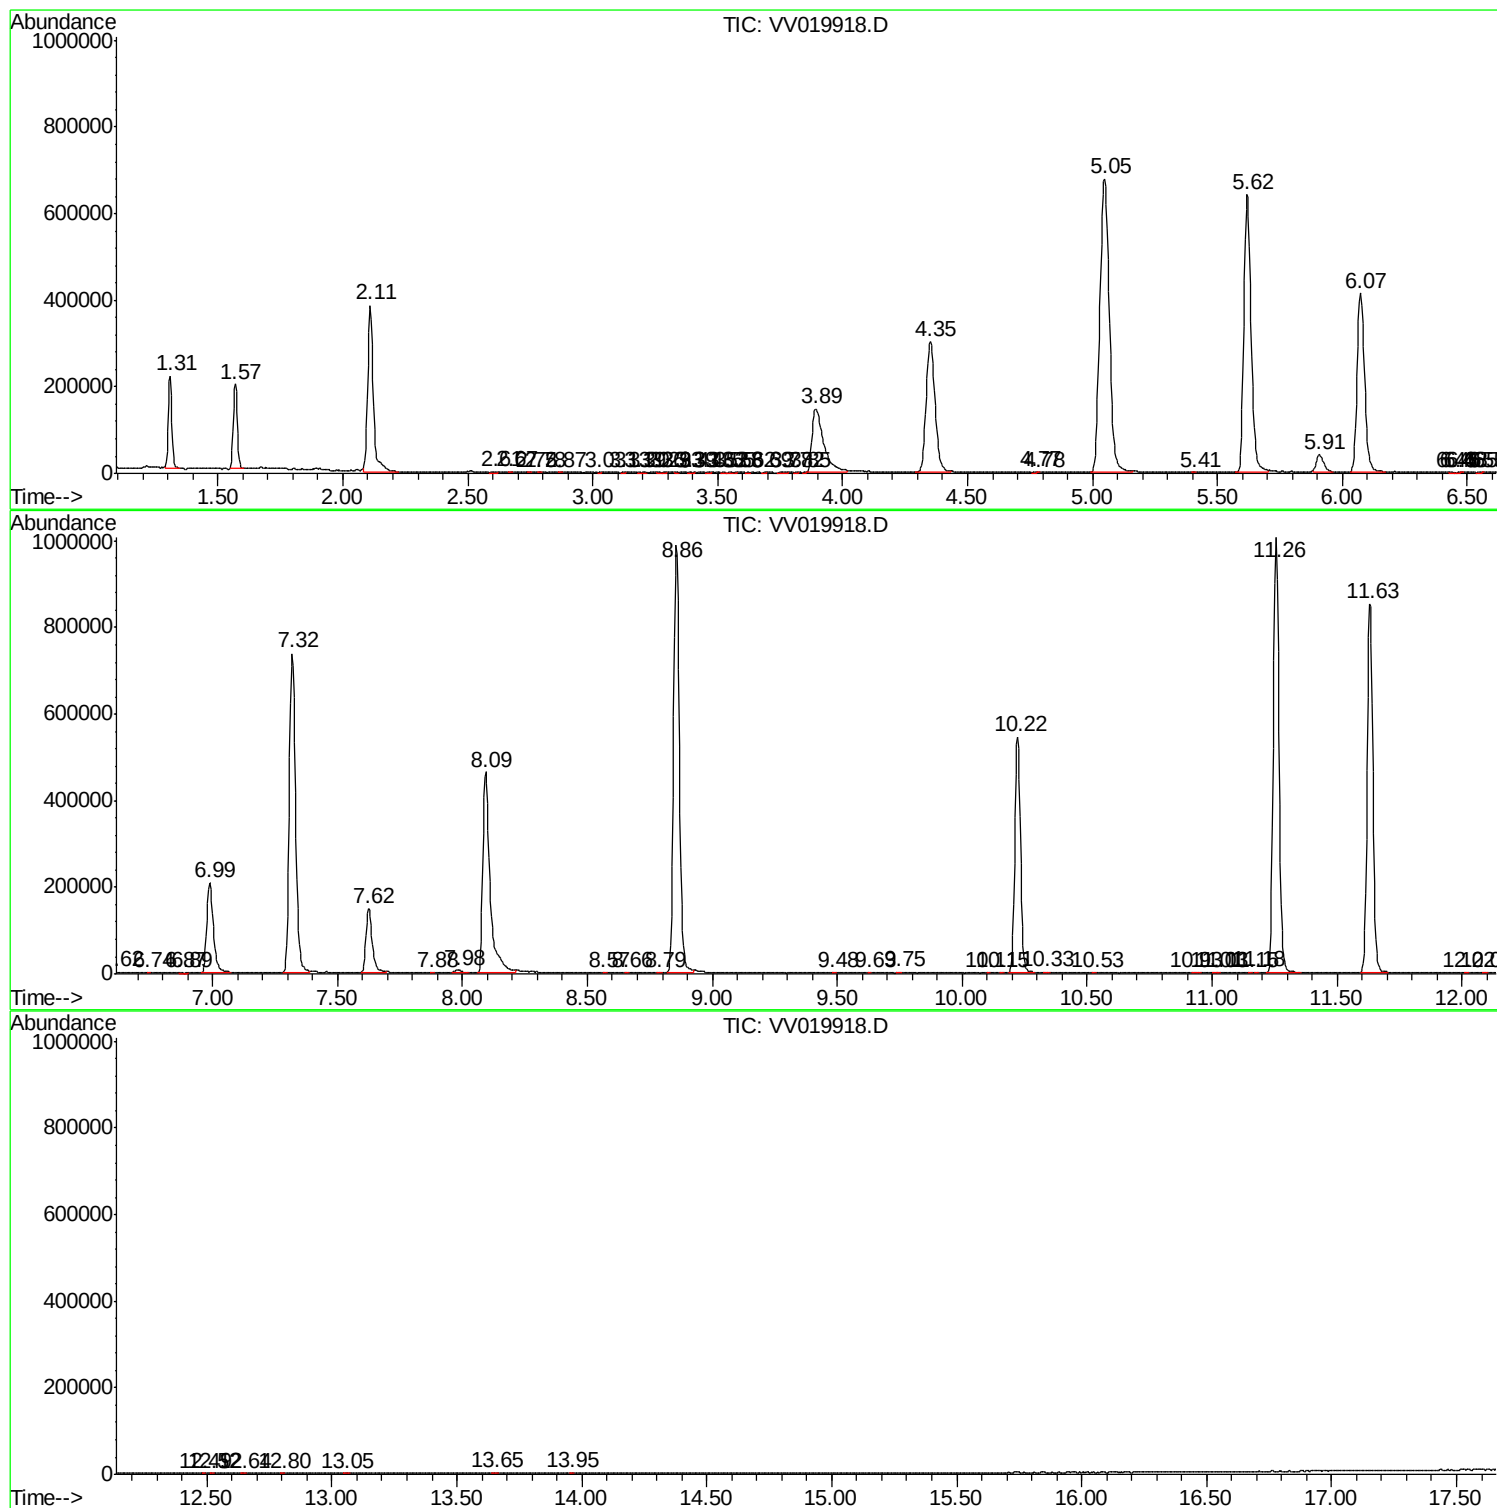

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010721\
Data File : VV019918.D
Acq On : 07 Jan 2021 13:35
Operator : SY/MD
Sample : M1016-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010721\
Data File : VV019918.D
Acq On : 07 Jan 2021 13:35
Operator : SY/MD
Sample : M1016-10 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4W8

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc