

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019926.D
 Acq On : 07 Jan 2021 17:01
 Operator : SY/MD
 Sample : M1017-05DL 400X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	196217	198098	8.88%	1.205%
2	1.569	143	149	159	rVB	186287	207499	9.30%	1.262%
3	2.110	308	317	346	rVB	362878	572557	25.67%	3.483%
4	2.508	435	441	450	rBV10	3056	5346	0.24%	0.033%
5	2.566	457	459	464	rBV5	785	806	0.04%	0.005%
6	2.717	503	506	508	rBV4	623	456	0.02%	0.003%
7	2.769	512	522	532	rVV4	8104	15655	0.70%	0.095%
8	2.872	550	554	558	rBV6	861	910	0.04%	0.006%
9	3.113	626	629	632	rBV3	953	571	0.03%	0.003%
10	3.135	635	636	639	rVB2	910	283	0.01%	0.002%
11	3.148	639	640	642	rBV2	541	210	0.01%	0.001%
12	3.180	647	650	652	rBV2	656	394	0.02%	0.002%
13	3.206	657	658	660	rBV2	602	284	0.01%	0.002%
14	3.277	677	680	684	rBV4	1412	1054	0.05%	0.006%
15	3.335	694	698	700	rBV3	1079	639	0.03%	0.004%
16	3.418	718	724	726	rBV4	1043	839	0.04%	0.005%
17	3.454	732	735	738	rVV5	590	376	0.02%	0.002%
18	3.499	747	749	751	rBV	644	384	0.02%	0.002%
19	3.576	768	773	776	rBV4	1541	1284	0.06%	0.008%
20	3.611	781	784	788	rBV3	1004	727	0.03%	0.004%
21	3.634	788	791	794	rBV3	1061	754	0.03%	0.005%
22	3.682	805	806	807	rBV3	752	204	0.01%	0.001%
23	3.727	819	820	826	rVB2	839	604	0.03%	0.004%
24	3.753	826	828	831	rBV2	625	496	0.02%	0.003%
25	3.897	861	873	909	rBV	154775	500652	22.44%	3.046%
26	4.354	1000	1015	1042	rBV	290108	706945	31.69%	4.301%
27	4.650	1105	1107	1108	rBV2	599	206	0.01%	0.001%
28	4.791	1148	1151	1153	rBV2	913	612	0.03%	0.004%
29	4.804	1153	1155	1156	rBV	870	409	0.02%	0.002%
30	4.881	1175	1179	1181	rBV4	490	389	0.02%	0.002%
31	4.965	1204	1205	1208	rBV2	593	385	0.02%	0.002%
32	5.052	1215	1232	1261	rBV2	664501	1707404	76.54%	10.388%
33	5.434	1349	1351	1353	rBV2	944	369	0.02%	0.002%
34	5.447	1353	1355	1356	rBV3	704	220	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019926.D
 Acq On : 07 Jan 2021 17:01
 Operator : SY/MD
 Sample : M1017-05DL 400X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	5.621	1397	1409	1434	rBV	617660	1232834	55.27%	7.500%
36	5.916	1490	1501	1523	rVB8	70565	164681	7.38%	1.002%
37	6.074	1536	1550	1573	rBV	404490	826263	37.04%	5.027%
38	6.392	1646	1649	1651	rVB5	1005	487	0.02%	0.003%
39	6.408	1651	1654	1655	rBV2	551	305	0.01%	0.002%
40	6.466	1669	1672	1673	rBV3	795	414	0.02%	0.003%
41	6.543	1694	1696	1699	rBV3	744	526	0.02%	0.003%
42	6.585	1707	1709	1710	rBV2	525	200	0.01%	0.001%
43	6.839	1785	1788	1790	rBV2	758	424	0.02%	0.003%
44	6.855	1790	1793	1797	rVV3	1236	969	0.04%	0.006%
45	6.875	1797	1799	1803	rVV4	781	556	0.02%	0.003%
46	6.897	1803	1806	1809	rVV3	808	542	0.02%	0.003%
47	6.952	1820	1823	1824	rBV3	724	353	0.02%	0.002%
48	6.990	1824	1835	1856	rBV	203839	370792	16.62%	2.256%
49	7.322	1925	1938	1965	rBV	711406	1242021	55.68%	7.556%
50	7.627	2023	2033	2052	rBV	135993	243441	10.91%	1.481%
51	7.859	2103	2105	2107	rBV2	862	498	0.02%	0.003%
52	7.894	2114	2116	2119	rBV4	1295	704	0.03%	0.004%
53	7.981	2129	2143	2164	rBV	1341710	2230619	100.00%	13.571%
54	8.093	2169	2178	2218	rVV2	478536	952413	42.70%	5.794%
55	8.785	2389	2393	2396	rBV5	848	684	0.03%	0.004%
56	8.855	2404	2415	2448	rBV	957538	1563137	70.08%	9.510%
57	9.164	2503	2511	2512	rBV7	1283	1392	0.06%	0.008%
58	9.260	2540	2541	2544	rBV3	807	344	0.02%	0.002%
59	9.321	2558	2560	2562	rVB2	1049	375	0.02%	0.002%
60	9.331	2562	2563	2566	rVB2	614	289	0.01%	0.002%
61	9.350	2566	2569	2570	rBV2	621	306	0.01%	0.002%
62	9.389	2578	2581	2584	rBV3	874	724	0.03%	0.004%
63	9.469	2604	2606	2610	rBV3	865	478	0.02%	0.003%
64	9.514	2618	2620	2624	rBV3	624	401	0.02%	0.002%
65	9.563	2632	2635	2639	rBV4	770	759	0.03%	0.005%
66	9.588	2640	2643	2645	rBV3	1177	663	0.03%	0.004%
67	9.714	2680	2682	2683	rBV2	590	227	0.01%	0.001%
68	9.826	2714	2717	2719	rBV3	838	461	0.02%	0.003%
69	9.884	2732	2735	2738	rBV4	900	548	0.02%	0.003%
70	9.939	2749	2752	2754	rBV	1060	620	0.03%	0.004%
71	10.003	2770	2772	2776	rBV3	689	588	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019926.D
 Acq On : 07 Jan 2021 17:01
 Operator : SY/MD
 Sample : M1017-05DL 400X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.138	2811	2814	2818	rBV3	1176	1024	0.05%	0.006%
73	10.222	2828	2840	2857	rBV	553455	864801	38.77%	5.261%
74	10.386	2888	2891	2900	rVB9	2629	3062	0.14%	0.019%
75	10.473	2911	2918	2921	rBV4	1004	1005	0.05%	0.006%
76	10.540	2937	2939	2941	rVB3	1006	412	0.02%	0.003%
77	10.563	2943	2946	2948	rVV4	951	573	0.03%	0.003%
78	10.678	2979	2982	2984	rBV3	725	330	0.01%	0.002%
79	10.701	2984	2989	2994	rBV5	1079	1366	0.06%	0.008%
80	10.739	3000	3001	3005	rVB4	846	500	0.02%	0.003%
81	10.807	3020	3022	3025	rVB4	910	417	0.02%	0.003%
82	10.855	3032	3037	3043	rBV6	1083	1055	0.05%	0.006%
83	10.887	3043	3047	3051	rBV6	1093	1085	0.05%	0.007%
84	10.968	3070	3072	3074	rBV3	725	391	0.02%	0.002%
85	11.145	3122	3127	3129	rVB3	759	609	0.03%	0.004%
86	11.170	3129	3135	3136	rBV2	963	835	0.04%	0.005%
87	11.257	3150	3162	3183	rBV	947969	1487562	66.69%	9.050%
88	11.633	3266	3279	3299	rBV	824236	1295705	58.09%	7.883%
89	11.987	3387	3389	3390	rBV	607	216	0.01%	0.001%
90	12.090	3417	3421	3422	rBV4	824	566	0.03%	0.003%
91	12.350	3500	3502	3504	rBV	781	436	0.02%	0.003%
92	12.379	3507	3511	3512	rBV3	1024	670	0.03%	0.004%
93	12.511	3550	3552	3554	rBV3	729	340	0.02%	0.002%
94	12.624	3584	3587	3590	rBV3	874	680	0.03%	0.004%
95	12.636	3590	3591	3592	rBV	769	247	0.01%	0.002%
96	12.884	3663	3668	3670	rBV3	920	799	0.04%	0.005%
97	13.128	3740	3744	3749	rBV5	1523	1331	0.06%	0.008%
98	13.431	3836	3838	3841	rBV3	1135	603	0.03%	0.004%
99	13.604	3890	3892	3896	rBV3	650	424	0.02%	0.003%
100	13.820	3957	3959	3963	rVB4	1342	860	0.04%	0.005%


Sum of corrected areas: 16436963

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010721\
Data File : VV019926.D
Acq On : 07 Jan 2021 17:01
Operator : SY/MD
Sample : M1017-05DL 400X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG4W5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

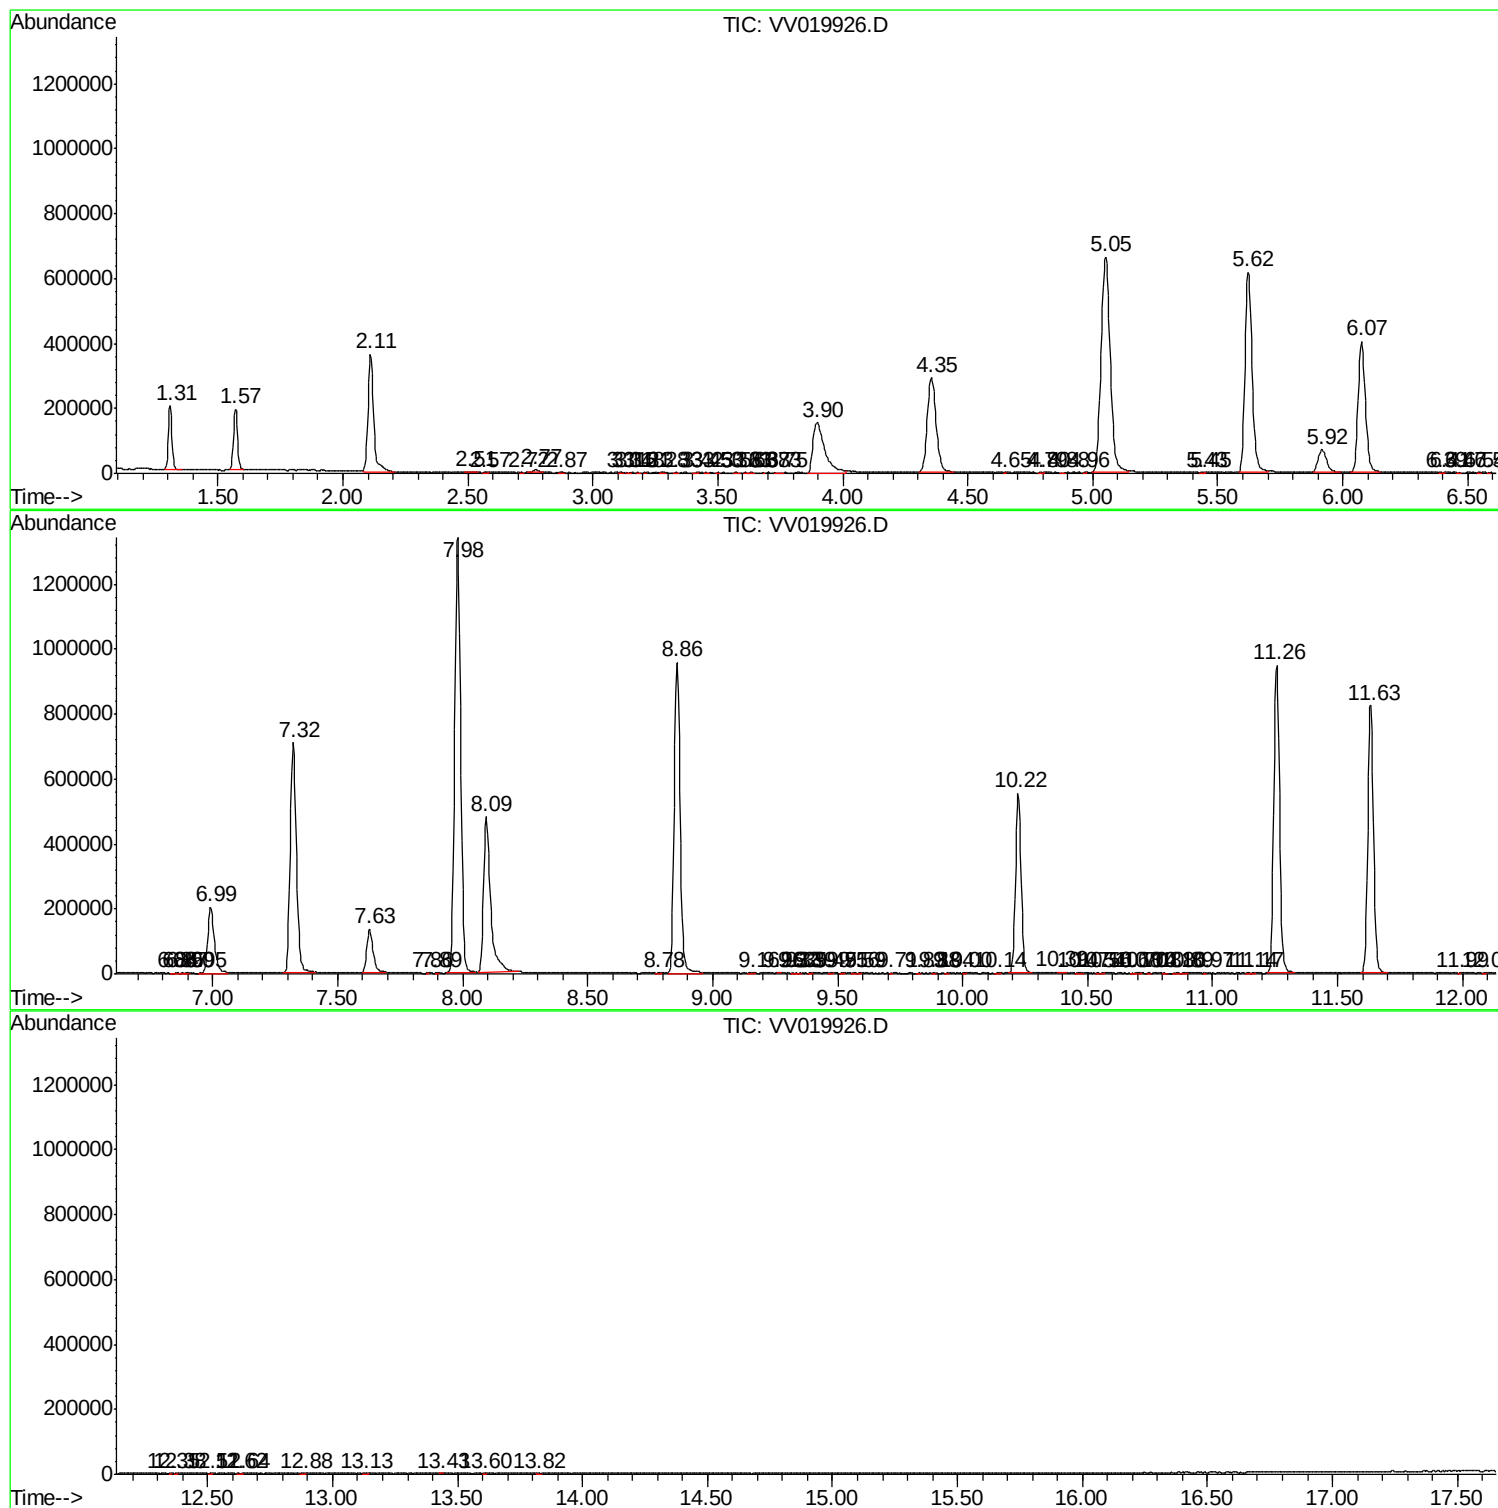

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010721\
Data File : VV019926.D
Acq On : 07 Jan 2021 17:01
Operator : SY/MD
Sample : M1017-05DL 400X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010721\
Data File : VV019926.D
Acq On : 07 Jan 2021 17:01
Operator : SY/MD
Sample : M1017-05DL 400X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4W5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc