

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019927.D
 Acq On : 07 Jan 2021 17:25
 Operator : SY/MD
 Sample : M1017-06DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	196501	201930	9.89%	1.254%
2	1.570	142	149	161	rBV	190156	212682	10.41%	1.321%
3	2.110	308	317	350	rVB	359259	578420	28.32%	3.592%
4	2.660	485	488	489	rBV2	744	361	0.02%	0.002%
5	2.676	489	493	495	rVV4	531	437	0.02%	0.003%
6	2.733	508	511	514	rBV4	1203	929	0.05%	0.006%
7	2.817	535	537	540	rVB3	602	281	0.01%	0.002%
8	2.859	548	550	554	rBV2	861	469	0.02%	0.003%
9	2.897	560	562	563	rBV2	786	384	0.02%	0.002%
10	2.991	588	591	592	rBV2	782	473	0.02%	0.003%
11	3.090	619	622	627	rBV5	1082	814	0.04%	0.005%
12	3.116	627	630	633	rBV4	798	608	0.03%	0.004%
13	3.168	643	646	647	rBV2	822	530	0.03%	0.003%
14	3.222	659	663	664	rBV3	779	532	0.03%	0.003%
15	3.277	677	680	683	rBV4	1232	814	0.04%	0.005%
16	3.325	692	695	697	rBV2	615	445	0.02%	0.003%
17	3.425	724	726	729	rVV2	544	297	0.01%	0.002%
18	3.447	729	733	737	rVB4	1067	999	0.05%	0.006%
19	3.476	737	742	743	rBV4	642	578	0.03%	0.004%
20	3.512	751	753	756	rBV3	615	400	0.02%	0.002%
21	3.553	763	766	767	rBV3	495	273	0.01%	0.002%
22	3.566	768	770	773	rVB3	1068	516	0.03%	0.003%
23	3.692	804	809	815	rVB5	846	684	0.03%	0.004%
24	3.727	817	820	821	rBV2	701	291	0.01%	0.002%
25	3.743	821	825	830	rVB4	1456	1060	0.05%	0.007%
26	3.772	831	834	836	rBV3	697	386	0.02%	0.002%
27	3.791	836	840	844	rVB5	944	723	0.04%	0.004%
28	3.827	849	851	859	rVB7	645	564	0.03%	0.004%
29	3.891	859	871	898	rBV	162689	477590	23.38%	2.966%
30	4.354	1001	1015	1045	rVB	286135	704223	34.47%	4.374%
31	4.907	1180	1187	1189	rBV3	682	741	0.04%	0.005%
32	4.958	1201	1203	1206	rBV4	810	502	0.02%	0.003%
33	5.052	1215	1232	1262	rBV2	649577	1687772	82.62%	10.482%
34	5.376	1331	1333	1337	rBV4	743	477	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019927.D
 Acq On : 07 Jan 2021 17:25
 Operator : SY/MD
 Sample : M1017-06DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	5.457	1354	1358	1359	rBV2	739	465	0.02%	0.003%
36	5.492	1367	1369	1372	rBV3	967	625	0.03%	0.004%
37	5.544	1383	1385	1389	rVB5	1278	833	0.04%	0.005%
38	5.569	1389	1393	1395	rBV2	1028	650	0.03%	0.004%
39	5.621	1395	1409	1438	rBV	618964	1255623	61.47%	7.798%
40	5.913	1490	1500	1518	rBV5	52412	118418	5.80%	0.735%
41	6.074	1536	1550	1573	rBV	404108	816811	39.99%	5.073%
42	6.389	1646	1648	1652	rBV4	805	517	0.03%	0.003%
43	6.476	1671	1675	1677	rVV4	1005	740	0.04%	0.005%
44	6.499	1680	1682	1685	rBV4	913	480	0.02%	0.003%
45	6.624	1718	1721	1722	rBV2	1410	874	0.04%	0.005%
46	6.759	1760	1763	1765	rBV4	1132	615	0.03%	0.004%
47	6.936	1814	1818	1820	rBV4	714	601	0.03%	0.004%
48	6.991	1824	1835	1857	rBV	192559	360045	17.63%	2.236%
49	7.322	1926	1938	1963	rBV	707370	1220899	59.77%	7.582%
50	7.627	2023	2033	2056	rBV	135882	240673	11.78%	1.495%
51	7.904	2117	2119	2122	rVB3	1054	356	0.02%	0.002%
52	7.923	2122	2125	2128	rBV2	844	607	0.03%	0.004%
53	7.981	2129	2143	2167	rBV	1225023	2042714	100.00%	12.686%
54	8.093	2168	2178	2212	rVV2	484512	948115	46.41%	5.888%
55	8.624	2341	2343	2345	rBV2	892	521	0.03%	0.003%
56	8.707	2363	2369	2374	rBV8	1372	1909	0.09%	0.012%
57	8.762	2382	2386	2390	rBV5	1166	1005	0.05%	0.006%
58	8.807	2398	2400	2402	rBV2	641	368	0.02%	0.002%
59	8.859	2403	2416	2439	rVV	954421	1567661	76.74%	9.736%
60	9.206	2522	2524	2527	rBV2	672	463	0.02%	0.003%
61	9.351	2565	2569	2571	rBV4	1014	925	0.05%	0.006%
62	9.396	2581	2583	2586	rBV3	751	515	0.03%	0.003%
63	9.543	2627	2629	2630	rBV2	682	279	0.01%	0.002%
64	9.579	2638	2640	2641	rBV2	777	303	0.01%	0.002%
65	9.617	2650	2652	2656	rBV4	1199	706	0.03%	0.004%
66	9.724	2683	2685	2689	rVV4	1222	804	0.04%	0.005%
67	9.814	2710	2713	2716	rBV4	854	629	0.03%	0.004%
68	9.871	2728	2731	2734	rBV3	857	575	0.03%	0.004%
69	9.897	2734	2739	2748	rVB7	1180	1330	0.07%	0.008%
70	9.936	2748	2751	2753	rBV3	1450	772	0.04%	0.005%
71	9.997	2767	2770	2774	rBV4	804	620	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019927.D
 Acq On : 07 Jan 2021 17:25
 Operator : SY/MD
 Sample : M1017-06DL 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4W6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.016	2774	2776	2781	rBV6	907	776	0.04%	0.005%
73	10.042	2782	2784	2785	rVV2	704	284	0.01%	0.002%
74	10.061	2788	2790	2791	rBV	741	331	0.02%	0.002%
75	10.145	2815	2816	2820	rBV2	377	320	0.02%	0.002%
76	10.177	2822	2826	2827	rBV4	530	300	0.01%	0.002%
77	10.222	2827	2840	2859	rBV	539662	858586	42.03%	5.332%
78	10.482	2917	2921	2922	rBV4	1476	870	0.04%	0.005%
79	10.540	2936	2939	2941	rBV3	1277	917	0.04%	0.006%
80	10.592	2951	2955	2957	rBV4	1028	886	0.04%	0.006%
81	10.688	2983	2985	2988	rBV2	1114	731	0.04%	0.005%
82	10.875	3041	3043	3045	rBV2	680	393	0.02%	0.002%
83	11.019	3084	3088	3091	rBV4	925	945	0.05%	0.006%
84	11.103	3110	3114	3116	rBV4	1302	833	0.04%	0.005%
85	11.145	3124	3127	3130	rBV3	813	741	0.04%	0.005%
86	11.257	3149	3162	3184	rBV	963571	1497142	73.29%	9.298%
87	11.630	3267	3278	3298	rBV	790449	1260113	61.69%	7.826%
88	11.762	3315	3319	3322	rBV5	1329	1110	0.05%	0.007%
89	11.830	3338	3340	3343	rBV4	827	563	0.03%	0.003%
90	11.920	3365	3368	3372	rVV3	1220	815	0.04%	0.005%
91	12.460	3534	3536	3539	rBV3	1106	676	0.03%	0.004%
92	12.569	3568	3570	3571	rBV	732	350	0.02%	0.002%
93	12.875	3663	3665	3669	rBV2	536	477	0.02%	0.003%
94	12.961	3689	3692	3695	rBV3	1060	650	0.03%	0.004%
95	13.090	3730	3732	3736	rVB2	1026	628	0.03%	0.004%
96	13.116	3737	3740	3742	rVV3	755	365	0.02%	0.002%
97	13.222	3768	3773	3775	rBV4	1260	1053	0.05%	0.007%
98	13.276	3786	3790	3796	rBV6	927	1252	0.06%	0.008%
99	13.669	3910	3912	3914	rBV2	754	307	0.02%	0.002%
100	14.421	4142	4146	4148	rBV3	1331	1076	0.05%	0.007%


Sum of corrected areas: 16101721

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010721\
Data File : VV019927.D
Acq On : 07 Jan 2021 17:25
Operator : SY/MD
Sample : M1017-06DL 1000X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

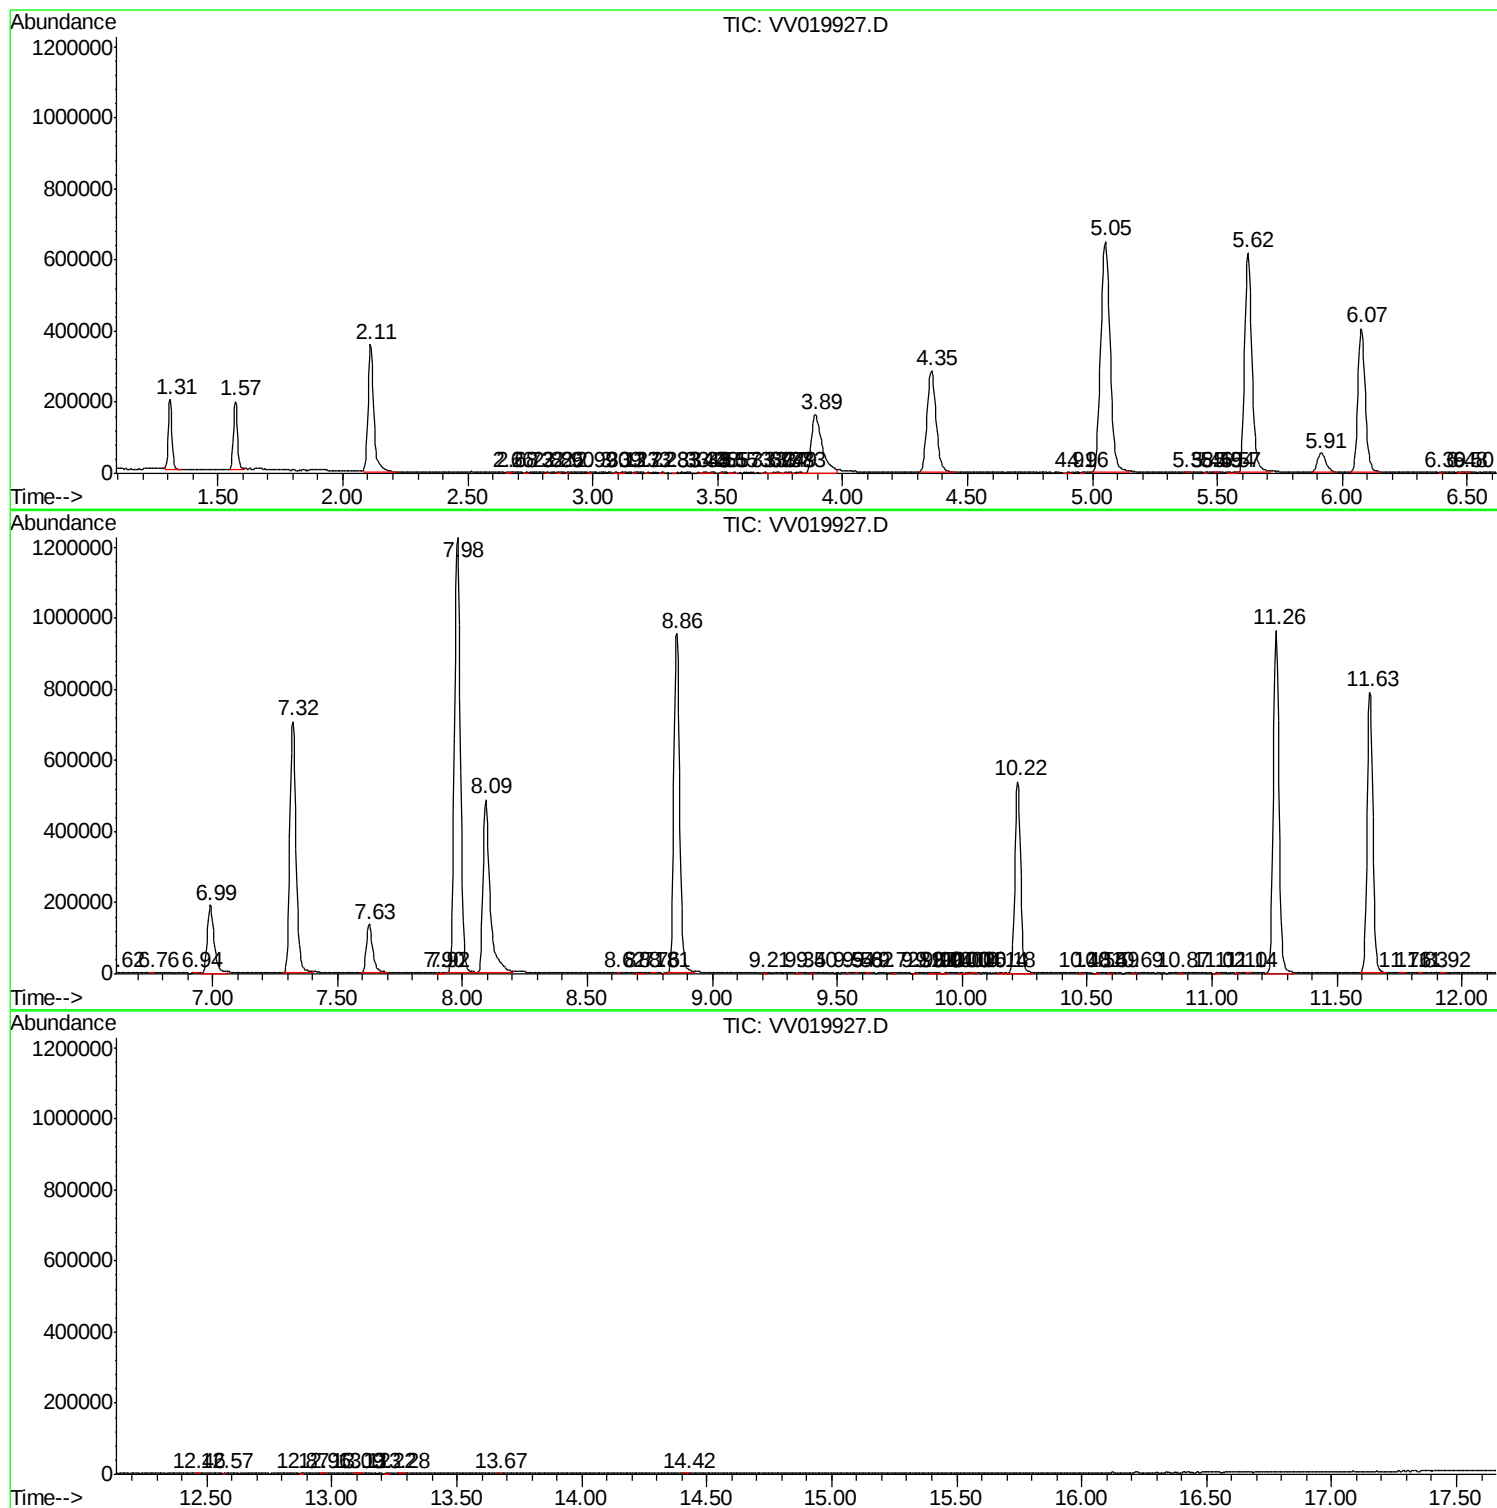

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010721\
Data File : VV019927.D
Acq On : 07 Jan 2021 17:25
Operator : SY/MD
Sample : M1017-06DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010721\
Data File : VV019927.D
Acq On : 07 Jan 2021 17:25
Operator : SY/MD
Sample : M1017-06DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4W6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc