

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019933.D
 Acq On : 07 Jan 2021 19:46
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	82	rVB	180010	179507	11.29%	1.341%
2	1.569	143	149	159	rVB	175762	193302	12.15%	1.444%
3	2.110	309	317	347	rVB	327978	527042	33.14%	3.936%
4	2.511	437	442	452	rVB7	3640	5304	0.33%	0.040%
5	2.566	457	459	461	rBV2	740	350	0.02%	0.003%
6	2.836	540	543	545	rBV2	693	452	0.03%	0.003%
7	2.904	562	564	565	rBV	443	120	0.01%	0.001%
8	2.955	579	580	582	rVB2	806	297	0.02%	0.002%
9	3.007	594	596	598	rBV3	1146	646	0.04%	0.005%
10	3.241	667	669	670	rBV2	929	307	0.02%	0.002%
11	3.318	691	693	694	rBV2	846	368	0.02%	0.003%
12	3.373	705	710	712	rBV4	896	705	0.04%	0.005%
13	3.495	746	748	750	rVB2	579	196	0.01%	0.001%
14	3.531	757	759	760	rBV3	466	226	0.01%	0.002%
15	3.553	764	766	767	rVB2	517	174	0.01%	0.001%
16	3.569	769	771	772	rBV2	433	134	0.01%	0.001%
17	3.630	788	790	791	rBV2	648	265	0.02%	0.002%
18	3.662	797	800	801	rBV3	1126	719	0.05%	0.005%
19	3.695	808	810	811	rBV2	1071	389	0.02%	0.003%
20	3.720	816	818	821	rVB3	1040	430	0.03%	0.003%
21	3.733	821	822	825	rBV2	816	399	0.03%	0.003%
22	3.765	830	832	834	rBV3	578	326	0.02%	0.002%
23	3.814	845	847	849	rBV3	523	318	0.02%	0.002%
24	3.888	859	870	902	rBV	164286	473157	29.75%	3.533%
25	4.354	1001	1015	1042	rVB	271420	668591	42.04%	4.993%
26	4.659	1108	1110	1117	rBV6	822	869	0.05%	0.006%
27	4.685	1117	1118	1122	rVB3	823	398	0.03%	0.003%
28	4.839	1164	1166	1170	rBV4	815	720	0.05%	0.005%
29	4.904	1184	1186	1189	rBV3	695	386	0.02%	0.003%
30	4.920	1189	1191	1195	rBV3	701	404	0.03%	0.003%
31	4.978	1207	1209	1212	rBV2	790	328	0.02%	0.002%
32	5.051	1214	1232	1258	rBV2	607279	1590427	100.00%	11.877%
33	5.524	1377	1379	1380	rBV2	657	232	0.01%	0.002%
34	5.621	1397	1409	1441	rBV	598642	1209809	76.07%	9.035%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019933.D
 Acq On : 07 Jan 2021 19:46
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	5.907	1489	1498	1519	rVB2	39416	81670	5.14%	0.610%
36	6.074	1537	1550	1575	rBV	377851	779162	48.99%	5.819%
37	6.563	1701	1702	1705	rBV3	752	453	0.03%	0.003%
38	6.598	1711	1713	1717	rBV3	727	537	0.03%	0.004%
39	6.804	1772	1777	1778	rBV4	1051	769	0.05%	0.006%
40	6.830	1783	1785	1788	rVB2	823	339	0.02%	0.003%
41	6.846	1788	1790	1796	rBV7	756	824	0.05%	0.006%
42	6.916	1808	1812	1814	rBV5	768	502	0.03%	0.004%
43	6.990	1824	1835	1859	rBV	185122	342189	21.52%	2.555%
44	7.322	1926	1938	1959	rBV	652267	1118910	70.35%	8.356%
45	7.582	2017	2019	2020	rBV2	839	355	0.02%	0.003%
46	7.627	2023	2033	2056	rVV	130605	232290	14.61%	1.735%
47	7.977	2139	2142	2144	rBV3	4197	3355	0.21%	0.025%
48	8.093	2166	2178	2215	rBV2	482239	973004	61.18%	7.266%
49	8.598	2333	2335	2336	rBV	534	184	0.01%	0.001%
50	8.691	2362	2364	2365	rBV	776	262	0.02%	0.002%
51	8.858	2404	2416	2441	rBV	926057	1505094	94.63%	11.240%
52	9.318	2554	2559	2561	rBV4	947	834	0.05%	0.006%
53	9.392	2579	2582	2589	rVB5	1074	1108	0.07%	0.008%
54	9.434	2593	2595	2598	rVB	811	376	0.02%	0.003%
55	9.498	2613	2615	2616	rBV	829	365	0.02%	0.003%
56	9.698	2674	2677	2680	rBV4	797	392	0.02%	0.003%
57	9.813	2711	2713	2714	rBV4	749	367	0.02%	0.003%
58	9.897	2736	2739	2740	rBV2	551	351	0.02%	0.003%
59	9.948	2752	2755	2758	rBV4	667	441	0.03%	0.003%
60	10.003	2768	2772	2774	rBV3	1069	778	0.05%	0.006%
61	10.100	2800	2802	2804	rBV3	910	407	0.03%	0.003%
62	10.141	2813	2815	2817	rBV2	872	385	0.02%	0.003%
63	10.222	2828	2840	2861	rBV	529768	832153	52.32%	6.214%
64	10.344	2875	2878	2881	rVB4	991	673	0.04%	0.005%
65	10.540	2937	2939	2940	rBV	874	369	0.02%	0.003%
66	10.591	2952	2955	2958	rBV4	1057	713	0.04%	0.005%
67	10.611	2958	2961	2963	rVV2	1046	552	0.03%	0.004%
68	10.727	2993	2997	2998	rBV2	638	372	0.02%	0.003%
69	10.762	3003	3008	3014	rBV4	1208	1361	0.09%	0.010%
70	10.823	3024	3027	3028	rBV2	727	336	0.02%	0.003%
71	10.865	3037	3040	3041	rBV3	1079	681	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010721\
 Data File : VV019933.D
 Acq On : 07 Jan 2021 19:46
 Operator : SY/MD
 Sample : VIBLK74
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.916	3054	3056	3061	rBV5	718	439	0.03%	0.003%
73	10.955	3065	3068	3070	rBV3	1079	826	0.05%	0.006%
74	10.977	3073	3075	3077	rBV3	554	293	0.02%	0.002%
75	11.016	3084	3087	3091	rBV5	1249	1075	0.07%	0.008%
76	11.128	3118	3122	3125	rBV5	678	642	0.04%	0.005%
77	11.170	3132	3135	3138	rBV5	824	841	0.05%	0.006%
78	11.254	3150	3161	3183	rBV	917643	1429529	89.88%	10.675%
79	11.582	3261	3263	3264	rBV2	864	293	0.02%	0.002%
80	11.630	3267	3278	3294	rVV	759870	1195612	75.18%	8.929%
81	12.353	3501	3503	3505	rBV2	908	471	0.03%	0.004%
82	12.405	3517	3519	3523	rBV3	877	604	0.04%	0.005%
83	12.553	3561	3565	3568	rBV4	1089	741	0.05%	0.006%
84	12.633	3587	3590	3593	rBV4	1289	801	0.05%	0.006%
85	12.739	3621	3623	3625	rBV2	969	415	0.03%	0.003%
86	12.916	3675	3678	3680	rBV2	884	563	0.04%	0.004%
87	13.032	3711	3714	3716	rBV3	997	658	0.04%	0.005%
88	13.749	3935	3937	3939	rBV2	928	322	0.02%	0.002%
89	13.759	3939	3940	3945	rVB3	1121	727	0.05%	0.005%
90	13.784	3945	3948	3950	rBV4	1130	884	0.06%	0.007%
91	14.160	4063	4065	4066	rBV2	967	473	0.03%	0.004%
92	14.289	4103	4105	4108	rBV2	1150	630	0.04%	0.005%
93	14.646	4213	4216	4217	rBV3	1219	762	0.05%	0.006%
94	16.443	4771	4775	4781	rVB	18355	12958	0.81%	0.097%


Sum of corrected areas: 13390769

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010721\
Data File : VV019933.D
Acq On : 07 Jan 2021 19:46
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

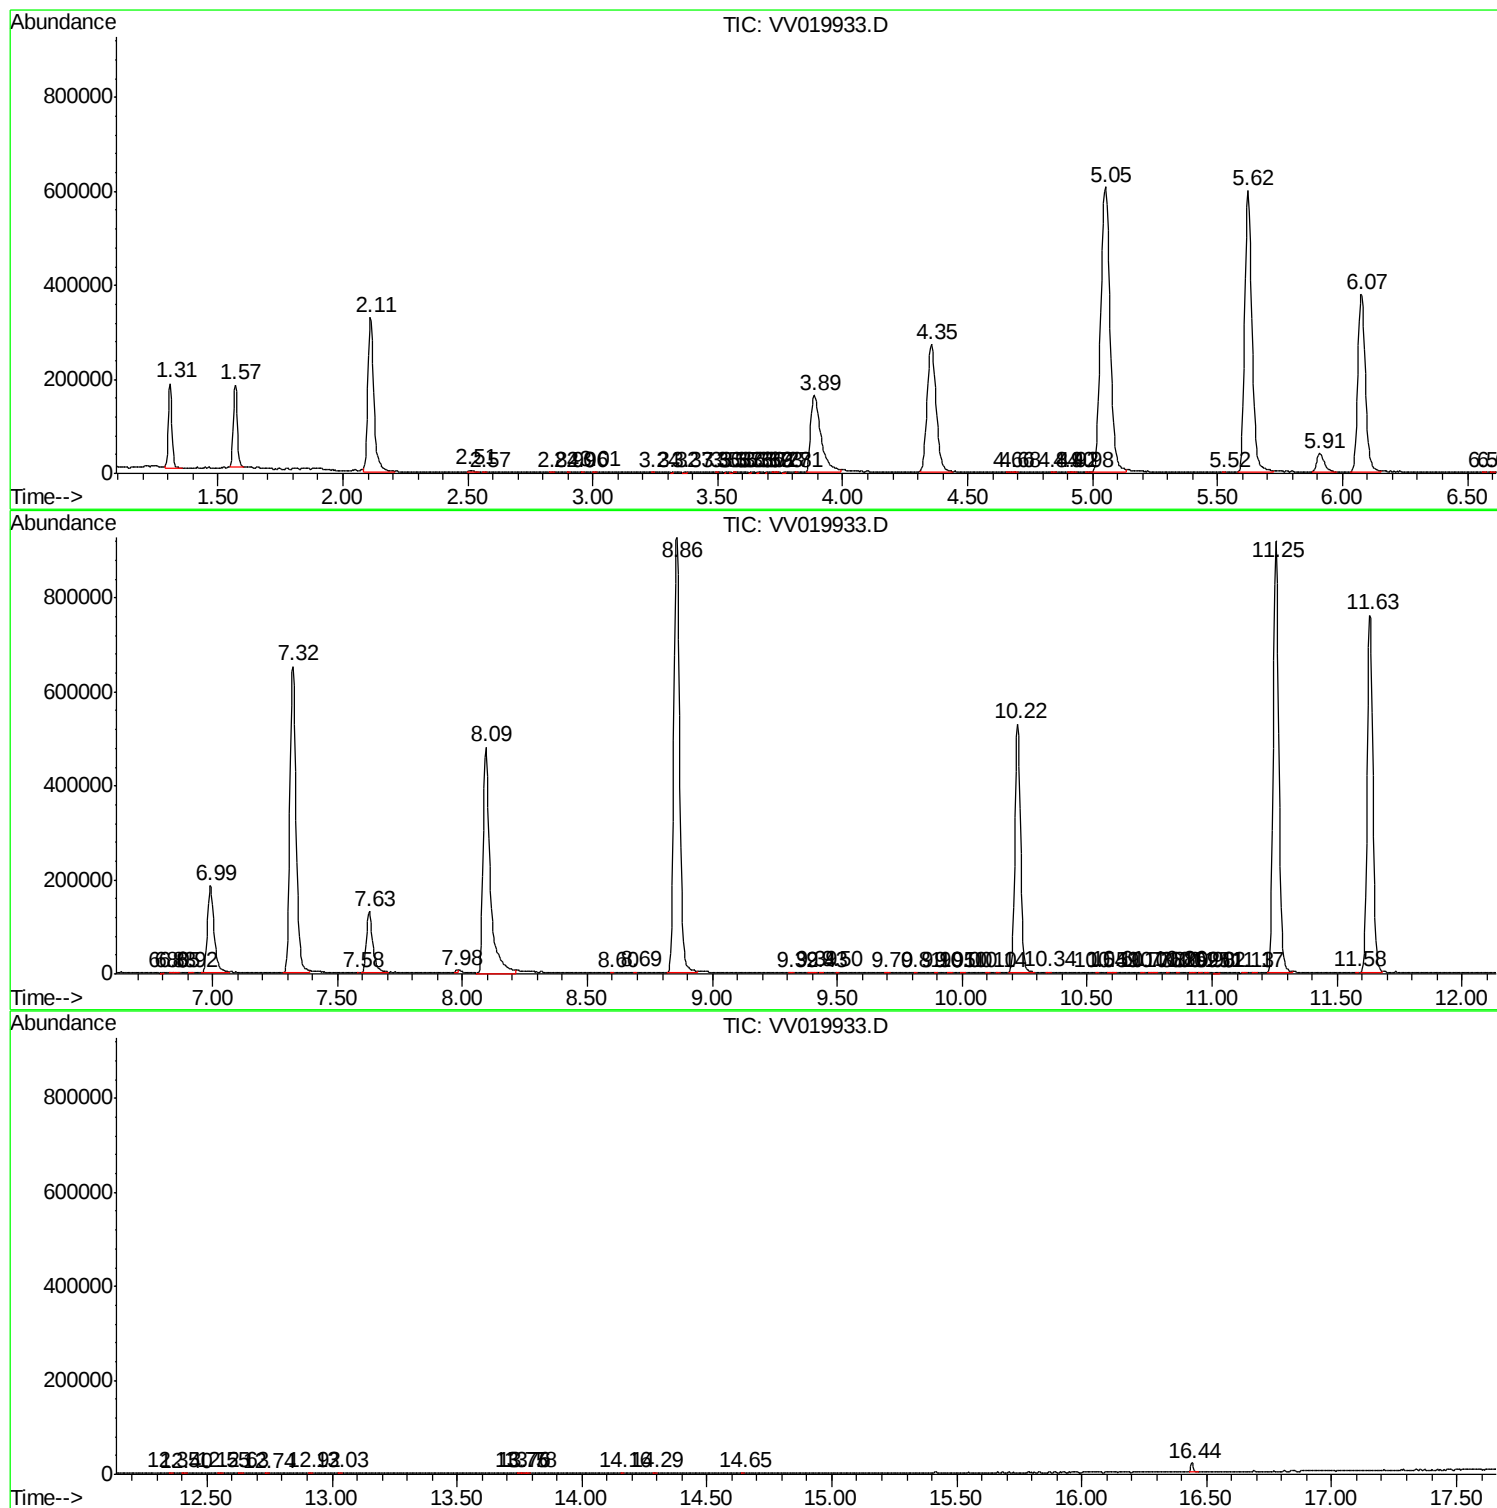

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010721\
Data File : VV019933.D
Acq On : 07 Jan 2021 19:46
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010721\
Data File : VV019933.D
Acq On : 07 Jan 2021 19:46
Operator : SY/MD
Sample : VIBLK74
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc