


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV010721\
 Data File : VV019911.D
 Acq On : 07 Jan 2021 08:52
 Operator : SY/MD
 Sample : BFB76
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB76

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 08 22:51:06 2021

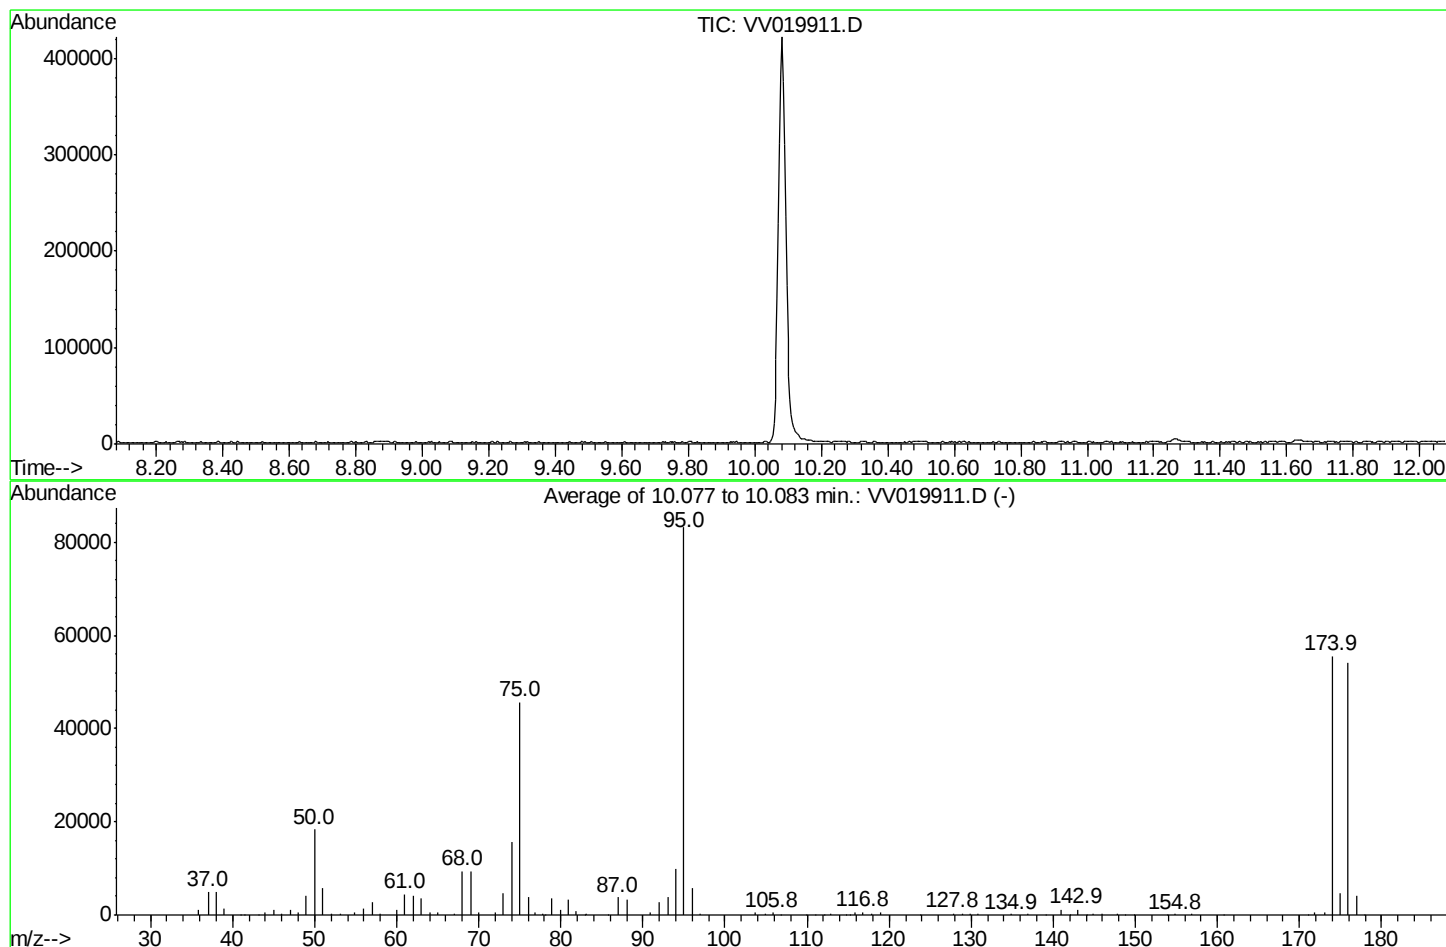

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	18320	PASS
75	95	30	80	55.0	45717	PASS
95	95	100	100	100.0	83168	PASS
96	95	5	9	7.0	5847	PASS
173	174	0.00	2	1.1	612	PASS
174	95	50	120	66.7	55509	PASS
175	174	5	9	8.4	4688	PASS
176	174	95	101	97.6	54178	PASS
177	176	5	9	7.4	4021	PASS

Scan 2784 (10.042 min): VV019911.D
BFB76

m/z	Abundance
39.10	121.0
39.90	294.0
42.00	106.0
44.00	755.0
45.30	115.0
51.10	108.0
86.70	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.90	988.0
37.00	4717.0
38.00	4889.0
39.00	1569.0
39.90	296.0
41.40	126.0
43.10	115.0
44.00	1372.0
45.00	1033.0
45.90	169.0
47.00	953.0
48.00	489.0
49.00	3879.0
50.00	17584.0
51.00	5458.0
52.00	277.0
53.10	146.0
54.90	394.0
56.00	1411.0
57.00	2778.0
58.00	183.0
60.00	915.0
61.00	4201.0
62.00	4002.0
63.00	3683.0
64.00	527.0
64.90	328.0
67.10	258.0
68.00	8954.0
69.00	8700.0
70.00	618.0
71.90	464.0
73.00	4341.0
74.00	15275.0
75.00	43520.0
76.00	3771.0
76.90	484.0
78.10	297.0
78.90	3442.0
79.90	1017.0
80.90	3377.0
81.90	801.0
82.90	180.0
85.60	104.0
86.90	3495.0
88.00	3049.0
90.90	506.0
92.00	2932.0
93.00	3557.0
94.00	9461.0
95.00	78432.0
96.00	5581.0
97.00	294.0
103.70	432.0
104.90	172.0
105.80	444.0
109.90	114.0
110.90	100.0
112.90	185.0
115.20	123.0
115.90	490.0
116.80	609.0
117.80	302.0
118.90	565.0
123.80	111.0
127.80	302.0
128.90	199.0
129.90	228.0
130.90	128.0
134.90	188.0
136.90	237.0
139.00	109.0
140.90	880.0
142.00	103.0
142.90	1087.0
144.00	126.0
144.80	167.0
145.90	141.0
147.80	202.0
148.80	153.0
149.90	118.0
154.80	154.0
156.80	173.0
160.80	110.0
171.80	431.0
173.00	834.0
173.90	50896.0
175.00	4340.0
176.00	49504.0
176.90	3759.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.90	1010.0
37.00	5267.0
38.00	5141.0
39.00	1638.0
39.90	272.0
41.40	131.0
44.00	1340.0
45.00	1035.0
46.00	186.0
47.00	1068.0
47.90	520.0
49.00	4206.0
50.00	18896.0
51.00	6206.0
52.00	339.0
53.10	172.0
54.90	443.0
56.00	1477.0
57.00	2971.0
57.90	150.0
59.90	1162.0
61.00	4510.0
62.00	4219.0
63.00	3783.0
64.00	491.0
65.00	484.0
67.10	257.0
68.00	9829.0
69.00	9653.0
70.00	669.0
71.90	484.0
73.00	4840.0
74.00	16158.0
75.00	47424.0
76.00	3965.0
76.90	567.0
77.80	397.0
78.90	3642.0
79.90	1097.0
80.90	3617.0
81.90	951.0
83.10	219.0
85.70	122.0
86.90	3977.0
88.00	3367.0
90.90	481.0
92.00	3042.0
93.00	4168.0
94.00	10197.0
95.00	86088.0
96.00	6111.0
97.00	330.0
103.80	455.0
104.90	228.0
105.80	534.0
106.90	115.0
109.80	122.0
110.90	137.0
112.90	204.0
115.20	143.0
115.90	510.0
116.80	637.0
117.90	314.0
118.90	646.0
123.80	107.0
127.80	288.0
128.90	205.0
129.90	234.0
130.80	163.0
134.90	205.0
136.90	247.0
140.90	1080.0
142.90	1195.0
144.00	144.0
144.80	188.0
145.90	153.0
147.80	229.0
149.90	149.0
154.90	185.0
156.90	200.0
160.80	121.0
171.00	115.0
171.80	447.0
173.10	1004.0
174.00	57536.0
175.00	4905.0
175.90	55952.0
176.90	4212.0
177.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.90	1007.0
37.00	5028.0
38.00	4905.0
39.00	1678.0
39.90	272.0
40.90	110.0
41.40	131.0
44.00	1212.0
45.00	930.0
46.00	198.0
47.00	1060.0
48.00	508.0
49.00	4159.0
50.00	18480.0
51.00	6304.0
52.00	393.0
53.10	155.0
54.90	486.0
56.00	1486.0
57.00	2831.0
57.90	148.0
59.90	1184.0
61.00	4495.0
62.00	4241.0
63.00	3665.0
64.00	467.0
65.00	618.0
66.90	228.0
68.00	9451.0
69.00	9515.0
70.00	640.0
72.00	497.0
73.00	4632.0
74.00	15923.0
75.00	46208.0
76.00	3891.0
76.90	554.0
77.80	492.0
78.90	3601.0
79.90	1038.0
80.90	3322.0
81.90	1028.0
83.10	227.0
85.80	118.0
87.00	3823.0
88.00	3347.0
90.80	415.0
92.00	2647.0
93.00	4169.0
94.00	9994.0
95.00	84984.0
96.00	5850.0
96.90	319.0
103.80	456.0
104.90	231.0
105.80	518.0
106.80	134.0
111.00	135.0
112.10	114.0
112.90	169.0
114.80	116.0
115.90	442.0
116.80	638.0
117.90	298.0
118.90	659.0
123.90	112.0
127.80	290.0
129.00	208.0
129.90	244.0
130.80	175.0
134.90	230.0
136.80	201.0
140.90	1167.0
142.90	1113.0
144.00	146.0
144.80	187.0
145.90	153.0
147.80	217.0
149.90	145.0
153.90	101.0
154.90	222.0
156.90	180.0
160.80	131.0
171.10	136.0
171.90	473.0
174.00	58096.0
175.00	4820.0
175.90	57080.0
176.90	4094.0
177.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76