
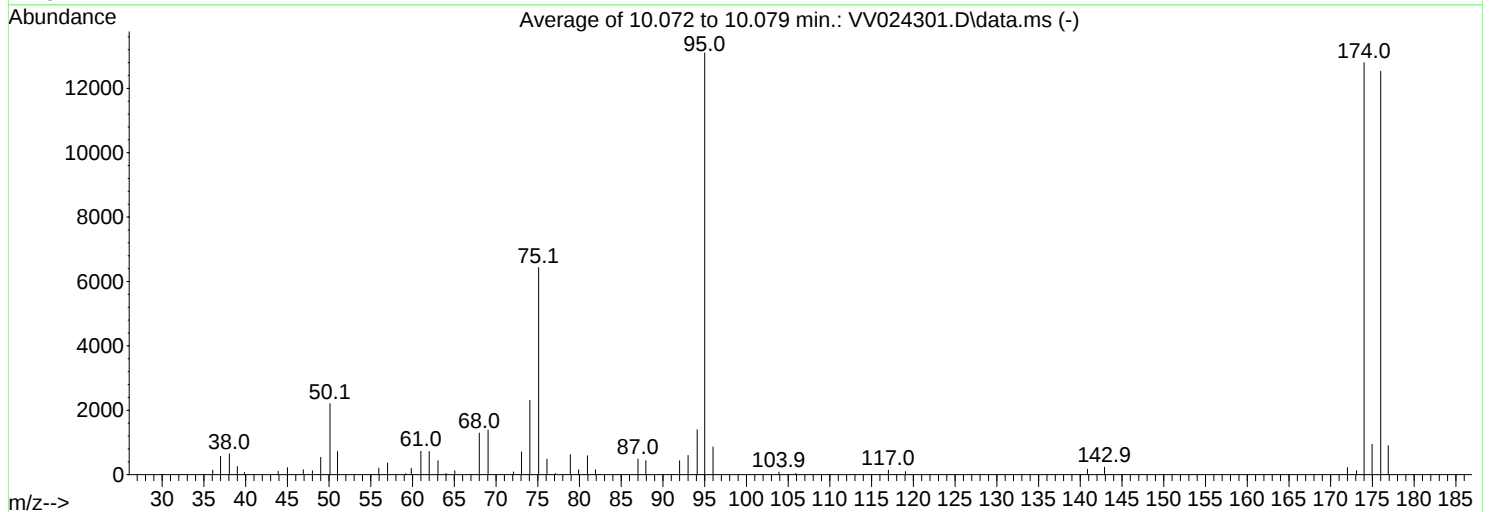


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010722\
 Data File : VV024301.D
 Acq On : 07 Jan 2022 10:14
 Operator : SY/MD
 Sample : BFB260
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB260

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Jan 11 01:51:56 2022

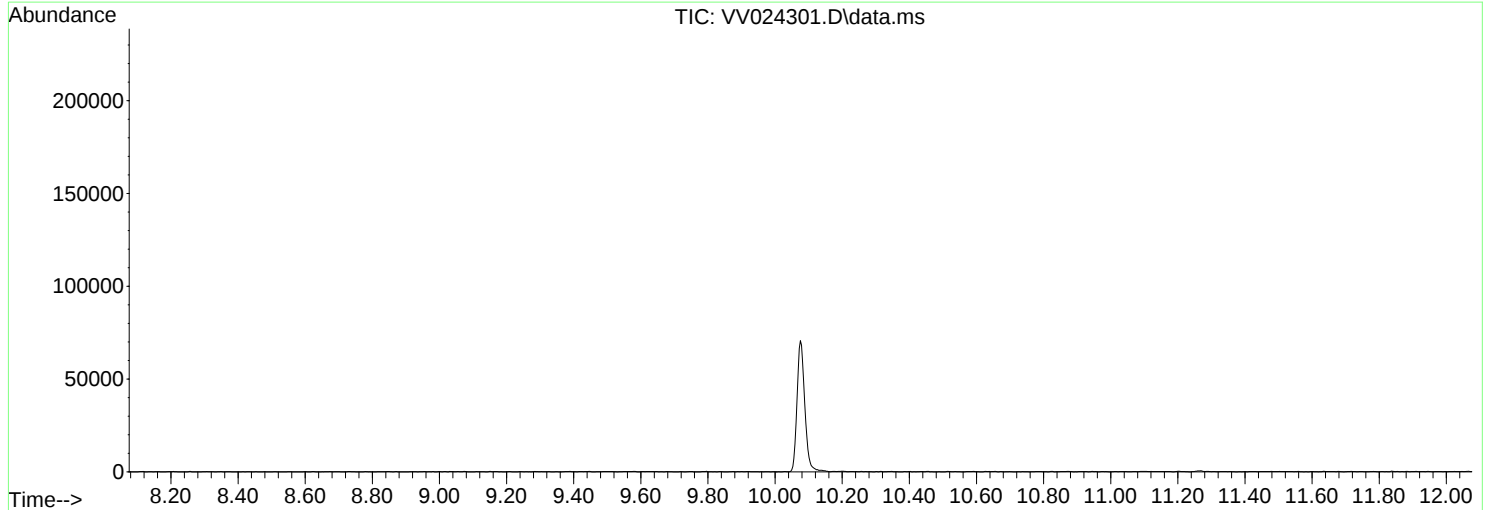

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	2206	PASS
75	95	30	80	49.1	6432	PASS
95	95	100	100	100.0	13102	PASS
96	95	5	9	6.6	860	PASS
173	174	0.00	2	1.0	126	PASS
174	95	50	120	97.7	12796	PASS
175	174	5	9	7.4	946	PASS
176	174	95	105	97.9	12530	PASS
177	176	5	10	7.2	902	PASS

m/z	Abundance
43.80	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
36.10	148.0
37.00	596.0
38.10	609.0
39.00	251.0
39.80	110.0
44.00	217.0
45.00	208.0
46.90	156.0
48.00	121.0
49.00	518.0
50.10	2206.0
51.00	728.0
56.00	232.0
57.00	373.0
59.20	100.0
59.90	213.0
61.00	734.0
62.00	641.0
63.10	418.0
65.10	122.0
68.00	1300.0
69.00	1342.0
73.10	676.0
74.00	2253.0
75.10	6385.0
76.10	522.0
78.90	630.0
80.00	138.0
81.00	569.0
82.00	127.0
87.00	492.0
87.90	471.0
92.00	425.0
93.00	572.0
94.10	1340.0
95.00	12961.0
96.00	751.0
117.00	105.0
119.10	160.0
140.80	152.0
142.90	213.0
172.00	179.0
173.10	175.0
174.00	11948.0
174.90	880.0
176.00	12165.0
176.90	848.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
36.00	133.0
37.00	561.0
38.00	693.0
39.00	266.0
44.00	237.0
45.00	240.0
46.90	161.0
48.00	124.0
49.00	565.0
50.10	2295.0
51.00	751.0
55.90	205.0
57.00	377.0
59.90	196.0
61.00	774.0
62.00	768.0
63.00	442.0
65.10	131.0
68.00	1335.0
69.10	1420.0
72.10	126.0
73.00	711.0
74.10	2386.0
75.10	6642.0
76.10	482.0
78.90	647.0
79.90	144.0
81.00	601.0
81.90	142.0
87.00	517.0
88.00	435.0
92.00	449.0
93.00	601.0
94.10	1399.0
95.00	13593.0
96.00	898.0
103.90	122.0
117.00	145.0
119.00	132.0
140.80	174.0
142.90	247.0
172.00	240.0
173.10	203.0
174.00	13142.0
175.00	971.0
176.00	12929.0
176.90	939.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
36.00	129.0
37.00	548.0
38.00	640.0
39.00	241.0
39.90	109.0
44.00	202.0
45.00	216.0
46.90	147.0
48.00	113.0
49.00	528.0
50.10	2116.0
51.00	666.0
55.90	174.0
57.00	339.0
59.80	168.0
61.00	670.0
62.00	753.0
63.00	445.0
64.00	116.0
64.90	114.0
68.00	1236.0
69.10	1406.0
72.10	131.0
73.00	725.0
74.10	2287.0
75.10	6270.0
76.10	438.0
77.10	104.0
78.90	580.0
79.80	164.0
80.90	593.0
81.80	172.0
87.00	449.0
88.00	390.0
92.00	422.0
93.00	612.0
94.10	1455.0
95.00	12751.0
96.00	930.0
103.90	117.0
105.90	107.0
117.00	170.0
140.90	188.0
142.90	247.0
172.00	231.0
174.00	13299.0
175.00	986.0
176.00	12496.0
176.90	918.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260