


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010819\
 Data File : VV009189.D
 Acq On : 08 Jan 2019 09:26
 Operator : SY/MD
 Sample : BFB70
 Misc : 5.00 G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB70

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM010819S.M
 Title : VOC Analysis
 Last Update : Wed Jan 09 00:40:20 2019

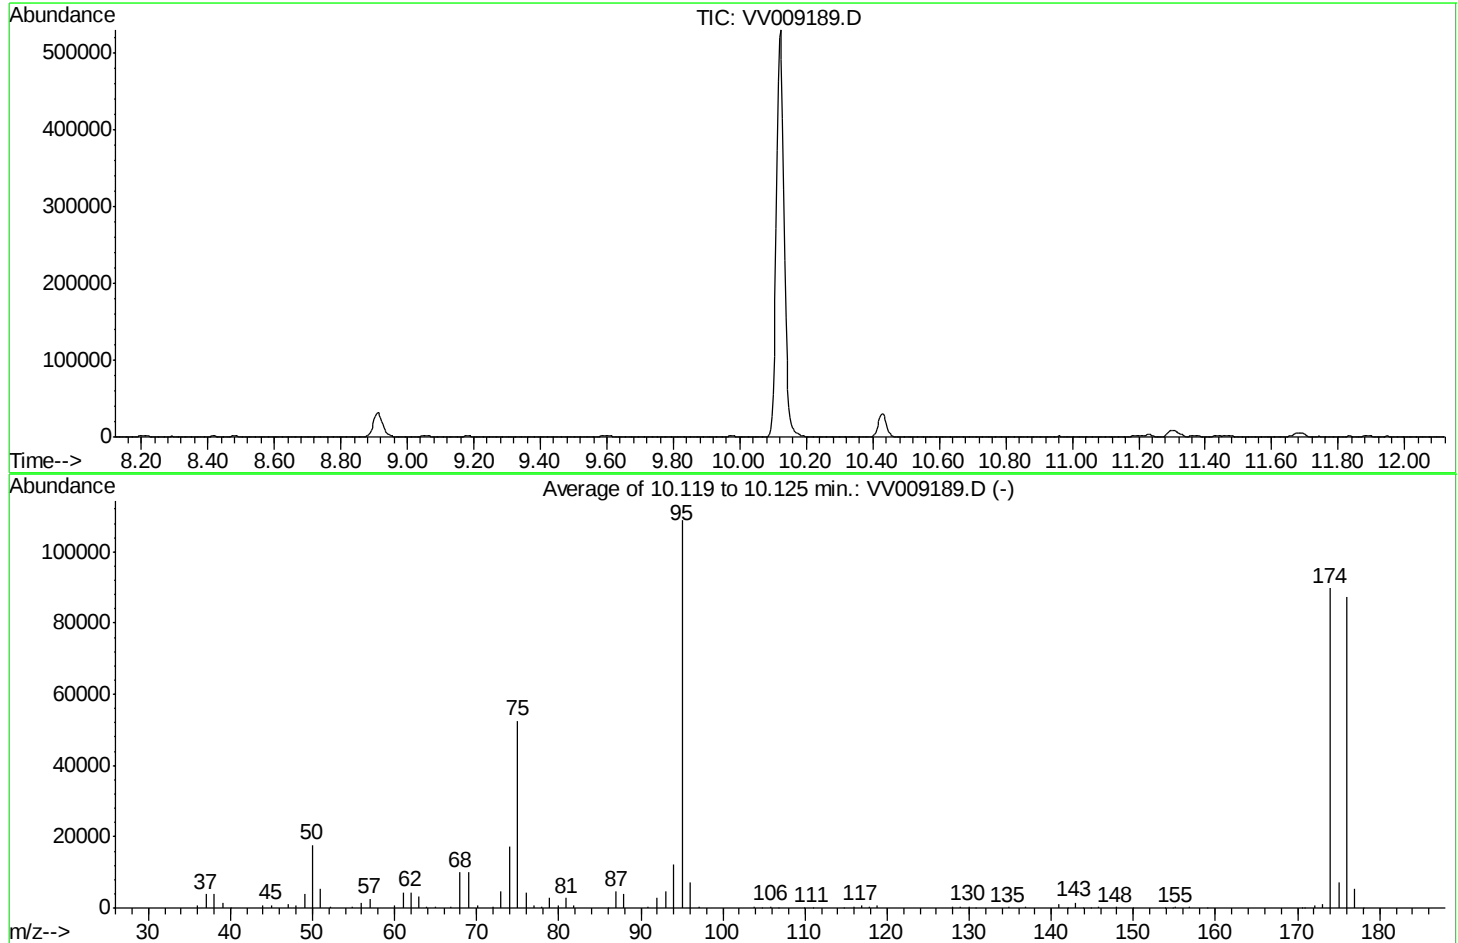

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	17657	PASS
75	95	30	80	48.2	52522	PASS
95	95	100	100	100.0	108866	PASS
96	95	5	9	6.6	7185	PASS
173	174	0.00	2	1.4	1224	PASS
174	95	50	120	82.4	89741	PASS
175	174	5	9	8.0	7189	PASS
176	174	95	101	97.3	87274	PASS
177	176	5	9	6.2	5413	PASS

m/z	Abundance
43.90	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	899.0
37.00	4083.0
38.00	4019.0
39.00	1488.0
40.00	203.0
44.00	733.0
45.00	788.0
47.00	1145.0
47.90	645.0
49.00	4400.0
50.00	18352.0
51.00	5861.0
52.10	185.0
54.90	277.0
56.00	1389.0
57.00	2634.0
60.00	869.0
61.00	4502.0
62.00	4628.0
63.00	3413.0
64.00	349.0
65.00	268.0
66.90	274.0
68.00	10176.0
69.00	10365.0
70.10	837.0
72.00	512.0
73.00	4754.0
74.00	17816.0
75.00	53224.0
76.00	4511.0
76.90	691.0
78.00	472.0
78.90	2890.0
80.00	843.0
80.90	2890.0
81.90	588.0
87.00	4534.0
87.90	4049.0
90.90	286.0
92.00	3086.0
93.00	4698.0
94.00	12525.0
95.00	111240.0
96.00	7241.0
97.20	251.0
103.80	464.0
104.70	149.0
105.90	525.0
106.70	119.0
110.90	125.0
114.80	131.0
115.90	393.0
116.90	697.0
117.90	458.0
118.80	625.0
127.90	341.0
128.80	190.0
130.00	375.0
130.90	170.0
134.80	235.0
136.80	261.0
140.90	1096.0
142.00	156.0
142.90	1482.0
143.90	119.0
144.80	151.0
145.80	211.0
147.80	281.0
150.00	177.0
155.10	261.0
156.90	199.0
170.50	108.0
170.90	147.0
172.00	614.0
173.10	1263.0
174.00	88144.0
175.00	7292.0
176.00	86800.0
177.00	5429.0
177.90	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	886.0
37.00	4030.0
38.00	3976.0
39.10	1487.0
40.00	176.0
44.00	780.0
45.00	762.0
47.00	1192.0
47.90	612.0
49.00	4246.0
50.00	18248.0
51.00	5724.0
52.10	207.0
54.90	232.0
56.00	1367.0
57.00	2712.0
60.00	920.0
61.00	4504.0
62.00	4676.0
63.00	3352.0
64.00	384.0
65.10	230.0
66.90	266.0
68.00	10262.0
69.00	10199.0
70.10	835.0
72.00	484.0
73.00	4650.0
74.00	17744.0
75.00	54200.0
76.00	4472.0
76.90	651.0
78.00	493.0
78.90	2974.0
79.90	838.0
80.90	2824.0
81.90	585.0
87.00	4686.0
87.90	4282.0
90.90	311.0
92.00	3168.0
93.00	4836.0
94.00	12624.0
95.00	112416.0
96.00	7411.0
97.10	215.0
103.90	427.0
104.80	135.0
105.90	478.0
106.80	112.0
109.90	101.0
114.70	150.0
116.00	446.0
116.90	650.0
117.80	491.0
118.80	678.0
127.90	389.0
128.90	212.0
129.90	383.0
130.80	143.0
134.80	241.0
136.80	233.0
140.90	1125.0
142.00	164.0
142.90	1548.0
144.80	141.0
145.80	251.0
147.90	302.0
150.00	134.0
155.10	250.0
156.80	194.0
159.00	103.0
170.90	146.0
172.00	608.0
173.10	1276.0
174.00	92712.0
175.00	7319.0
176.00	89984.0
177.00	5567.0
178.00	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	792.0
37.00	3579.0
38.00	3615.0
39.10	1315.0
39.90	160.0
44.00	714.0
44.90	720.0
47.00	1072.0
48.00	533.0
49.00	3608.0
50.00	16372.0
51.00	5131.0
52.20	213.0
54.90	211.0
56.00	1164.0
57.00	2581.0
60.00	813.0
61.00	4215.0
62.00	4204.0
63.00	3078.0
63.90	397.0
65.10	231.0
66.90	225.0
68.00	9422.0
69.00	9137.0
70.00	715.0
72.00	416.0
73.00	4239.0
74.00	16000.0
75.00	50144.0
76.00	4022.0
77.00	531.0
77.90	454.0
78.90	2829.0
79.90	828.0
81.00	2631.0
81.80	583.0
86.00	139.0
87.00	4451.0
88.00	3959.0
90.90	310.0
92.00	2883.0
93.00	4421.0
94.00	11659.0
95.00	102944.0
96.10	6903.0
97.00	168.0
103.90	432.0
104.80	107.0
105.90	401.0
106.80	105.0
114.70	151.0
116.00	445.0
116.90	603.0
117.80	441.0
118.80	630.0
127.90	366.0
128.90	220.0
129.90	354.0
130.80	127.0
134.80	218.0
136.90	186.0
140.90	1036.0
142.00	123.0
142.90	1405.0
144.70	116.0
145.80	257.0
147.90	278.0
149.80	117.0
153.80	106.0
154.80	216.0
155.20	220.0
156.90	188.0
170.90	104.0
172.10	616.0
173.10	1135.0
174.00	88368.0
175.00	6958.0
176.00	85040.0
177.00	5243.0
178.10	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70