

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019939.D
 Acq On : 08 Jan 2021 10:56
 Operator : SY/MD
 Sample : VV0108WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	268015	268123	13.20%	1.710%
2	1.569	142	149	162	rVB	233974	266479	13.12%	1.700%
3	2.110	308	317	343	rVB	461140	713786	35.13%	4.553%
4	2.286	367	372	375	rBV7	1795	1844	0.09%	0.012%
5	2.466	426	428	433	rBV3	795	507	0.02%	0.003%
6	2.505	433	440	441	rBV5	2429	2632	0.13%	0.017%
7	2.569	458	460	463	rBV2	1149	668	0.03%	0.004%
8	2.647	481	484	485	rBV2	780	477	0.02%	0.003%
9	2.865	549	552	553	rBV2	623	311	0.02%	0.002%
10	2.949	575	578	582	rBV2	1358	730	0.04%	0.005%
11	2.981	585	588	590	rBV2	499	379	0.02%	0.002%
12	3.016	597	599	601	rBV3	689	339	0.02%	0.002%
13	3.071	613	616	619	rVB3	1089	664	0.03%	0.004%
14	3.106	624	627	631	rBV4	795	785	0.04%	0.005%
15	3.171	645	647	652	rVV3	677	361	0.02%	0.002%
16	3.193	652	654	657	rVV2	468	235	0.01%	0.001%
17	3.254	669	673	676	rBV4	900	598	0.03%	0.004%
18	3.293	683	685	687	rVB3	1066	464	0.02%	0.003%
19	3.312	687	691	692	rBV3	731	513	0.03%	0.003%
20	3.399	715	718	721	rBV3	783	514	0.03%	0.003%
21	3.489	743	746	748	rVB5	1012	517	0.03%	0.003%
22	3.544	761	763	765	rBV2	454	253	0.01%	0.002%
23	3.576	770	773	774	rBV2	1277	676	0.03%	0.004%
24	3.621	783	787	788	rBV2	569	380	0.02%	0.002%
25	3.643	792	794	798	rVB3	1026	675	0.03%	0.004%
26	3.682	804	806	809	rBV2	632	305	0.02%	0.002%
27	3.704	809	813	814	rBV2	559	303	0.01%	0.002%
28	3.775	831	835	840	rBV6	741	730	0.04%	0.005%
29	3.807	843	845	846	rBV	505	265	0.01%	0.002%
30	3.891	860	871	908	rBV	163324	507503	24.98%	3.237%
31	4.354	1000	1015	1042	rVB	332481	816730	40.20%	5.210%
32	4.618	1094	1097	1100	rVB3	1307	675	0.03%	0.004%
33	4.717	1123	1128	1131	rBV7	1017	921	0.05%	0.006%
34	4.782	1144	1148	1152	rBV3	1313	937	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019939.D
 Acq On : 08 Jan 2021 10:56
 Operator : SY/MD
 Sample : VV0108WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	4.804	1152	1155	1157	rBV3	822	508	0.03%	0.003%
36	4.859	1166	1172	1173	rBV4	1061	1042	0.05%	0.007%
37	5.052	1214	1232	1258	rBV2	787496	2031609	100.00%	12.960%
38	5.537	1380	1383	1384	rBV3	581	332	0.02%	0.002%
39	5.621	1396	1409	1431	rBV	634602	1259631	62.00%	8.035%
40	5.910	1490	1499	1517	rVB3	39568	79329	3.90%	0.506%
41	6.074	1536	1550	1569	rBV	471382	946487	46.59%	6.038%
42	6.437	1661	1663	1665	rBV2	607	344	0.02%	0.002%
43	6.470	1671	1673	1674	rBV2	752	334	0.02%	0.002%
44	6.515	1685	1687	1689	rBV2	776	295	0.01%	0.002%
45	6.550	1696	1698	1701	rBV2	710	535	0.03%	0.003%
46	6.601	1709	1714	1717	rBV5	970	997	0.05%	0.006%
47	6.778	1767	1769	1773	rVB3	1365	692	0.03%	0.004%
48	6.888	1799	1803	1806	rBV3	782	621	0.03%	0.004%
49	6.916	1809	1812	1814	rBV2	836	504	0.02%	0.003%
50	6.929	1814	1816	1820	rBV4	1114	591	0.03%	0.004%
51	6.990	1823	1835	1855	rBV	249617	450623	22.18%	2.875%
52	7.322	1925	1938	1965	rBV	871269	1520858	74.86%	9.702%
53	7.627	2023	2033	2047	rBV	170944	294385	14.49%	1.878%
54	7.897	2114	2117	2121	rBV3	1085	831	0.04%	0.005%
55	8.093	2168	2178	2211	rBV2	520903	1033023	50.85%	6.590%
56	8.547	2316	2319	2322	rBV4	1108	892	0.04%	0.006%
57	8.752	2381	2383	2384	rBV	597	265	0.01%	0.002%
58	8.858	2403	2416	2445	rBV	967924	1580370	77.79%	10.081%
59	9.277	2544	2546	2547	rBV2	737	289	0.01%	0.002%
60	9.370	2573	2575	2577	rBV2	1029	463	0.02%	0.003%
61	9.428	2589	2593	2596	rBV4	838	477	0.02%	0.003%
62	9.476	2607	2608	2612	rVB4	1152	622	0.03%	0.004%
63	9.502	2612	2616	2617	rBV3	548	385	0.02%	0.002%
64	9.621	2649	2653	2654	rBV3	658	477	0.02%	0.003%
65	9.727	2683	2686	2690	rVB5	1125	661	0.03%	0.004%
66	9.768	2696	2699	2702	rBV4	829	469	0.02%	0.003%
67	9.936	2747	2751	2752	rBV3	831	533	0.03%	0.003%
68	10.042	2781	2784	2790	rVB4	1489	1281	0.06%	0.008%
69	10.077	2790	2795	2798	rBV5	1177	1241	0.06%	0.008%
70	10.106	2802	2804	2808	rBV3	819	492	0.02%	0.003%
71	10.222	2829	2840	2862	rVB	587248	904187	44.51%	5.768%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019939.D
 Acq On : 08 Jan 2021 10:56
 Operator : SY/MD
 Sample : VV0108WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.428	2900	2904	2907	rBV4	981	793	0.04%	0.005%
73	10.637	2967	2969	2970	rBV2	695	337	0.02%	0.002%
74	10.714	2991	2993	2995	rBV3	1008	560	0.03%	0.004%
75	10.833	3027	3030	3033	rBV3	854	678	0.03%	0.004%
76	10.926	3057	3059	3061	rBV3	979	471	0.02%	0.003%
77	10.993	3076	3080	3081	rBV3	723	571	0.03%	0.004%
78	11.016	3085	3087	3091	rVV5	1033	580	0.03%	0.004%
79	11.080	3105	3107	3109	rBV2	845	452	0.02%	0.003%
80	11.116	3113	3118	3120	rBV3	765	659	0.03%	0.004%
81	11.132	3120	3123	3125	rBV2	859	471	0.02%	0.003%
82	11.257	3149	3162	3185	rBV	973688	1506587	74.16%	9.611%
83	11.485	3231	3233	3239	rBV5	1012	607	0.03%	0.004%
84	11.633	3266	3279	3295	rBV	913067	1443794	71.07%	9.210%
85	12.009	3394	3396	3399	rBV3	871	482	0.02%	0.003%
86	12.051	3405	3409	3411	rBV3	1378	1150	0.06%	0.007%
87	12.090	3417	3421	3424	rBV4	1101	959	0.05%	0.006%
88	12.247	3467	3470	3473	rVB4	1145	691	0.03%	0.004%
89	12.264	3473	3475	3479	rBV3	800	676	0.03%	0.004%
90	12.350	3500	3502	3505	rBV2	648	281	0.01%	0.002%
91	12.376	3508	3510	3513	rBV2	829	600	0.03%	0.004%
92	12.421	3520	3524	3527	rBV4	826	808	0.04%	0.005%
93	12.456	3531	3535	3538	rBV4	803	857	0.04%	0.005%
94	12.762	3625	3630	3633	rBV5	880	842	0.04%	0.005%
95	12.878	3665	3666	3669	rBV	825	413	0.02%	0.003%
96	13.138	3744	3747	3749	rBV2	999	630	0.03%	0.004%
97	13.694	3917	3920	3924	rBV2	1135	882	0.04%	0.006%
98	13.717	3924	3927	3931	rBV3	707	712	0.04%	0.005%
99	14.103	4045	4047	4049	rBV2	1059	659	0.03%	0.004%
100	14.392	4134	4137	4143	rBV4	1255	1156	0.06%	0.007%


Sum of corrected areas: 15676312

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010821\
Data File : VV019939.D
Acq On : 08 Jan 2021 10:56
Operator : SY/MD
Sample : VV0108WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

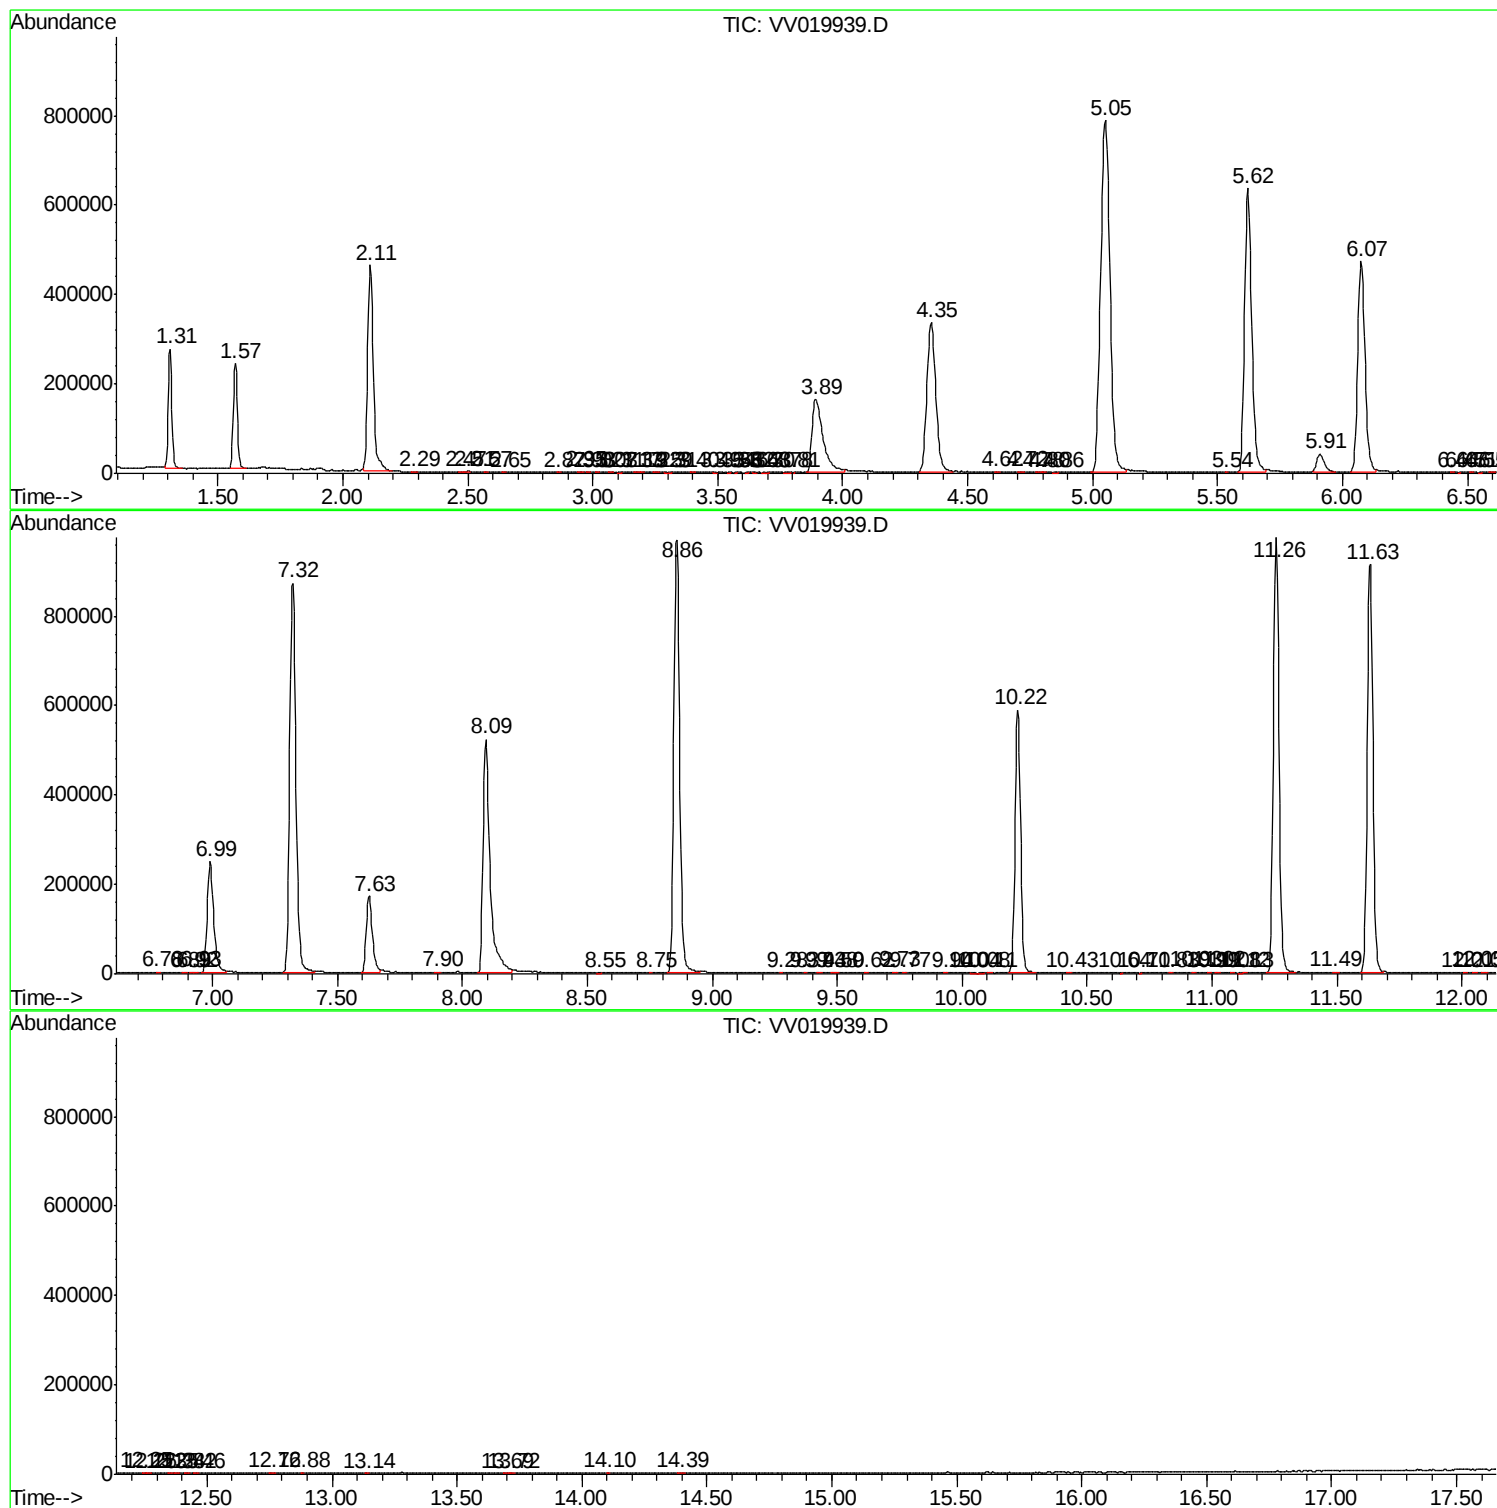

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019939.D
Acq On : 08 Jan 2021 10:56
Operator : SY/MD
Sample : VV0108WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019939.D
Acq On : 08 Jan 2021 10:56
Operator : SY/MD
Sample : VV0108WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc