

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019941.D
 Acq On : 08 Jan 2021 12:35
 Operator : SY/MD
 Sample : M1053-01ME
 Misc : 6.21g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFN59ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.306	61	67	87	rVB	141022	189986	10.74%	1.345%
2	1.563	142	147	161	rBV	111871	172128	9.73%	1.219%
3	2.084	300	309	319	rBV	360788	511276	28.90%	3.621%
4	3.004	592	595	598	rBV4	1342	1172	0.07%	0.008%
5	3.161	641	644	646	rBV3	856	652	0.04%	0.005%
6	3.174	646	648	649	rVV	575	214	0.01%	0.002%
7	3.338	694	699	701	rBV3	1187	1077	0.06%	0.008%
8	3.364	705	707	709	rVV3	933	429	0.02%	0.003%
9	3.396	713	717	723	rBV4	1157	1050	0.06%	0.007%
10	3.425	723	726	727	rBV2	836	472	0.03%	0.003%
11	3.544	759	763	764	rBV	642	394	0.02%	0.003%
12	3.579	769	774	777	rBV4	898	821	0.05%	0.006%
13	3.653	795	797	799	rBV2	823	433	0.02%	0.003%
14	3.737	820	823	825	rBV3	985	638	0.04%	0.005%
15	3.756	825	829	830	rVV2	724	547	0.03%	0.004%
16	3.788	833	839	841	rBV5	1157	1172	0.07%	0.008%
17	3.827	845	851	854	rBV6	1278	1428	0.08%	0.010%
18	3.894	861	872	900	rBV	95063	364719	20.62%	2.583%
19	4.344	998	1012	1038	rVB	275519	718068	40.59%	5.085%
20	4.605	1092	1093	1099	rVB4	1260	556	0.03%	0.004%
21	4.836	1163	1165	1168	rVB2	719	407	0.02%	0.003%
22	4.894	1180	1183	1184	rBV2	829	443	0.03%	0.003%
23	4.913	1187	1189	1191	rBV2	708	287	0.02%	0.002%
24	4.942	1195	1198	1202	rBV3	653	502	0.03%	0.004%
25	5.039	1211	1228	1262	rBV2	700656	1769097	100.00%	12.528%
26	5.614	1392	1407	1440	rBV	631347	1355938	76.65%	9.602%
27	5.904	1489	1497	1515	rVB2	37899	80554	4.55%	0.570%
28	6.068	1536	1548	1573	rVB	386420	828471	46.83%	5.867%
29	6.325	1626	1628	1631	rVB4	1414	822	0.05%	0.006%
30	6.454	1667	1668	1671	rBV3	667	449	0.03%	0.003%
31	6.511	1684	1686	1689	rBV2	751	484	0.03%	0.003%
32	6.592	1709	1711	1713	rVB2	828	269	0.02%	0.002%
33	6.608	1713	1716	1717	rBV2	1418	730	0.04%	0.005%
34	6.646	1717	1728	1730	rBV8	3021	5244	0.30%	0.037%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019941.D
 Acq On : 08 Jan 2021 12:35
 Operator : SY/MD
 Sample : M1053-01ME
 Misc : 6.21g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFN59ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	6.708	1745	1747	1750	rBV4	1195	726	0.04%	0.005%
36	6.933	1814	1817	1819	rBV3	825	635	0.04%	0.004%
37	6.987	1823	1834	1860	rVV	179710	373518	21.11%	2.645%
38	7.257	1916	1918	1920	rBV3	1004	617	0.03%	0.004%
39	7.315	1925	1936	1961	rVV	698060	1263746	71.43%	8.950%
40	7.624	2022	2032	2057	rBV	116902	250807	14.18%	1.776%
41	7.913	2120	2122	2124	rBV2	764	320	0.02%	0.002%
42	8.064	2164	2169	2170	rBV3	973	707	0.04%	0.005%
43	8.126	2171	2188	2226	rVV2	311229	918491	51.92%	6.505%
44	8.698	2360	2366	2370	rBV5	992	1030	0.06%	0.007%
45	8.724	2370	2374	2376	rVB4	946	583	0.03%	0.004%
46	8.740	2376	2379	2381	rBV3	664	404	0.02%	0.003%
47	8.794	2395	2396	2398	rBV2	766	323	0.02%	0.002%
48	8.859	2404	2416	2438	rBV	858972	1634539	92.39%	11.575%
49	9.212	2523	2526	2529	rBV4	802	580	0.03%	0.004%
50	9.254	2537	2539	2541	rVB3	734	192	0.01%	0.001%
51	9.363	2570	2573	2577	rBV3	877	741	0.04%	0.005%
52	9.428	2591	2593	2595	rBV	525	293	0.02%	0.002%
53	9.450	2595	2600	2602	rBV3	954	998	0.06%	0.007%
54	9.489	2609	2612	2614	rBV2	1488	790	0.04%	0.006%
55	9.518	2619	2621	2622	rBV	892	394	0.02%	0.003%
56	9.637	2656	2658	2659	rBV2	795	405	0.02%	0.003%
57	9.656	2662	2664	2667	rVV2	977	468	0.03%	0.003%
58	9.743	2689	2691	2696	rBV3	1269	876	0.05%	0.006%
59	9.769	2696	2699	2700	rBV2	858	498	0.03%	0.004%
60	9.849	2722	2724	2725	rBV2	1079	370	0.02%	0.003%
61	9.894	2735	2738	2741	rBV2	1155	892	0.05%	0.006%
62	9.929	2747	2749	2754	rBV4	1021	733	0.04%	0.005%
63	9.952	2754	2756	2757	rBV	823	315	0.02%	0.002%
64	10.084	2794	2797	2798	rBV3	866	476	0.03%	0.003%
65	10.170	2821	2824	2827	rBV5	853	685	0.04%	0.005%
66	10.228	2830	2842	2860	rVV	481362	827582	46.78%	5.861%
67	10.379	2884	2889	2891	rBV5	1846	1868	0.11%	0.013%
68	10.415	2898	2900	2904	rVB3	1186	804	0.05%	0.006%
69	10.434	2904	2906	2910	rBV2	541	429	0.02%	0.003%
70	10.463	2912	2915	2918	rVB3	598	452	0.03%	0.003%
71	10.521	2928	2933	2936	rBV6	769	746	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019941.D
 Acq On : 08 Jan 2021 12:35
 Operator : SY/MD
 Sample : M1053-01ME
 Misc : 6.21g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFN59ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.537	2936	2938	2940	rVB3	552	224	0.01%	0.002%
73	10.550	2940	2942	2943	rBV2	1106	457	0.03%	0.003%
74	10.781	3009	3014	3019	rBV5	1533	1802	0.10%	0.013%
75	10.852	3033	3036	3038	rBV3	805	418	0.02%	0.003%
76	11.029	3087	3091	3094	rBV3	1472	1179	0.07%	0.008%
77	11.071	3101	3104	3107	rBV4	1589	1051	0.06%	0.007%
78	11.260	3151	3163	3179	rBV	987679	1536727	86.87%	10.883%
79	11.637	3267	3280	3299	rBV	801227	1257028	71.05%	8.902%
80	11.926	3368	3370	3372	rBV3	739	379	0.02%	0.003%
81	12.000	3389	3393	3396	rBV4	961	833	0.05%	0.006%
82	12.051	3407	3409	3412	rBV5	671	334	0.02%	0.002%
83	12.138	3430	3436	3439	rBV6	1312	1401	0.08%	0.010%
84	12.215	3457	3460	3465	rVB5	972	713	0.04%	0.005%
85	12.254	3466	3472	3480	rBV2	4184	6700	0.38%	0.047%
86	12.412	3518	3521	3527	rBV6	1367	1194	0.07%	0.008%
87	12.537	3557	3560	3563	rBV3	607	488	0.03%	0.003%
88	12.572	3569	3571	3573	rBV	678	273	0.02%	0.002%
89	12.659	3593	3598	3602	rBV7	1706	1989	0.11%	0.014%
90	12.916	3675	3678	3683	rBV3	855	950	0.05%	0.007%
91	12.968	3692	3694	3700	rVB4	910	698	0.04%	0.005%
92	13.141	3742	3748	3752	rBV6	1159	1160	0.07%	0.008%
93	13.183	3760	3761	3764	rBV	768	445	0.03%	0.003%
94	13.231	3774	3776	3779	rBV3	587	296	0.02%	0.002%
95	13.270	3784	3788	3789	rBV	1615	1115	0.06%	0.008%
96	13.309	3798	3800	3805	rBV5	771	706	0.04%	0.005%
97	13.360	3812	3816	3820	rBV6	850	878	0.05%	0.006%
98	13.392	3824	3826	3828	rBV3	878	480	0.03%	0.003%
99	13.511	3859	3863	3865	rBV3	1846	1320	0.07%	0.009%
100	14.225	4083	4085	4089	rBV3	702	568	0.03%	0.004%


Sum of corrected areas: 14120768

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010821\
Data File : VV019941.D
Acq On : 08 Jan 2021 12:35
Operator : SY/MD
Sample : M1053-01ME
Misc : 6.21g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFN59ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

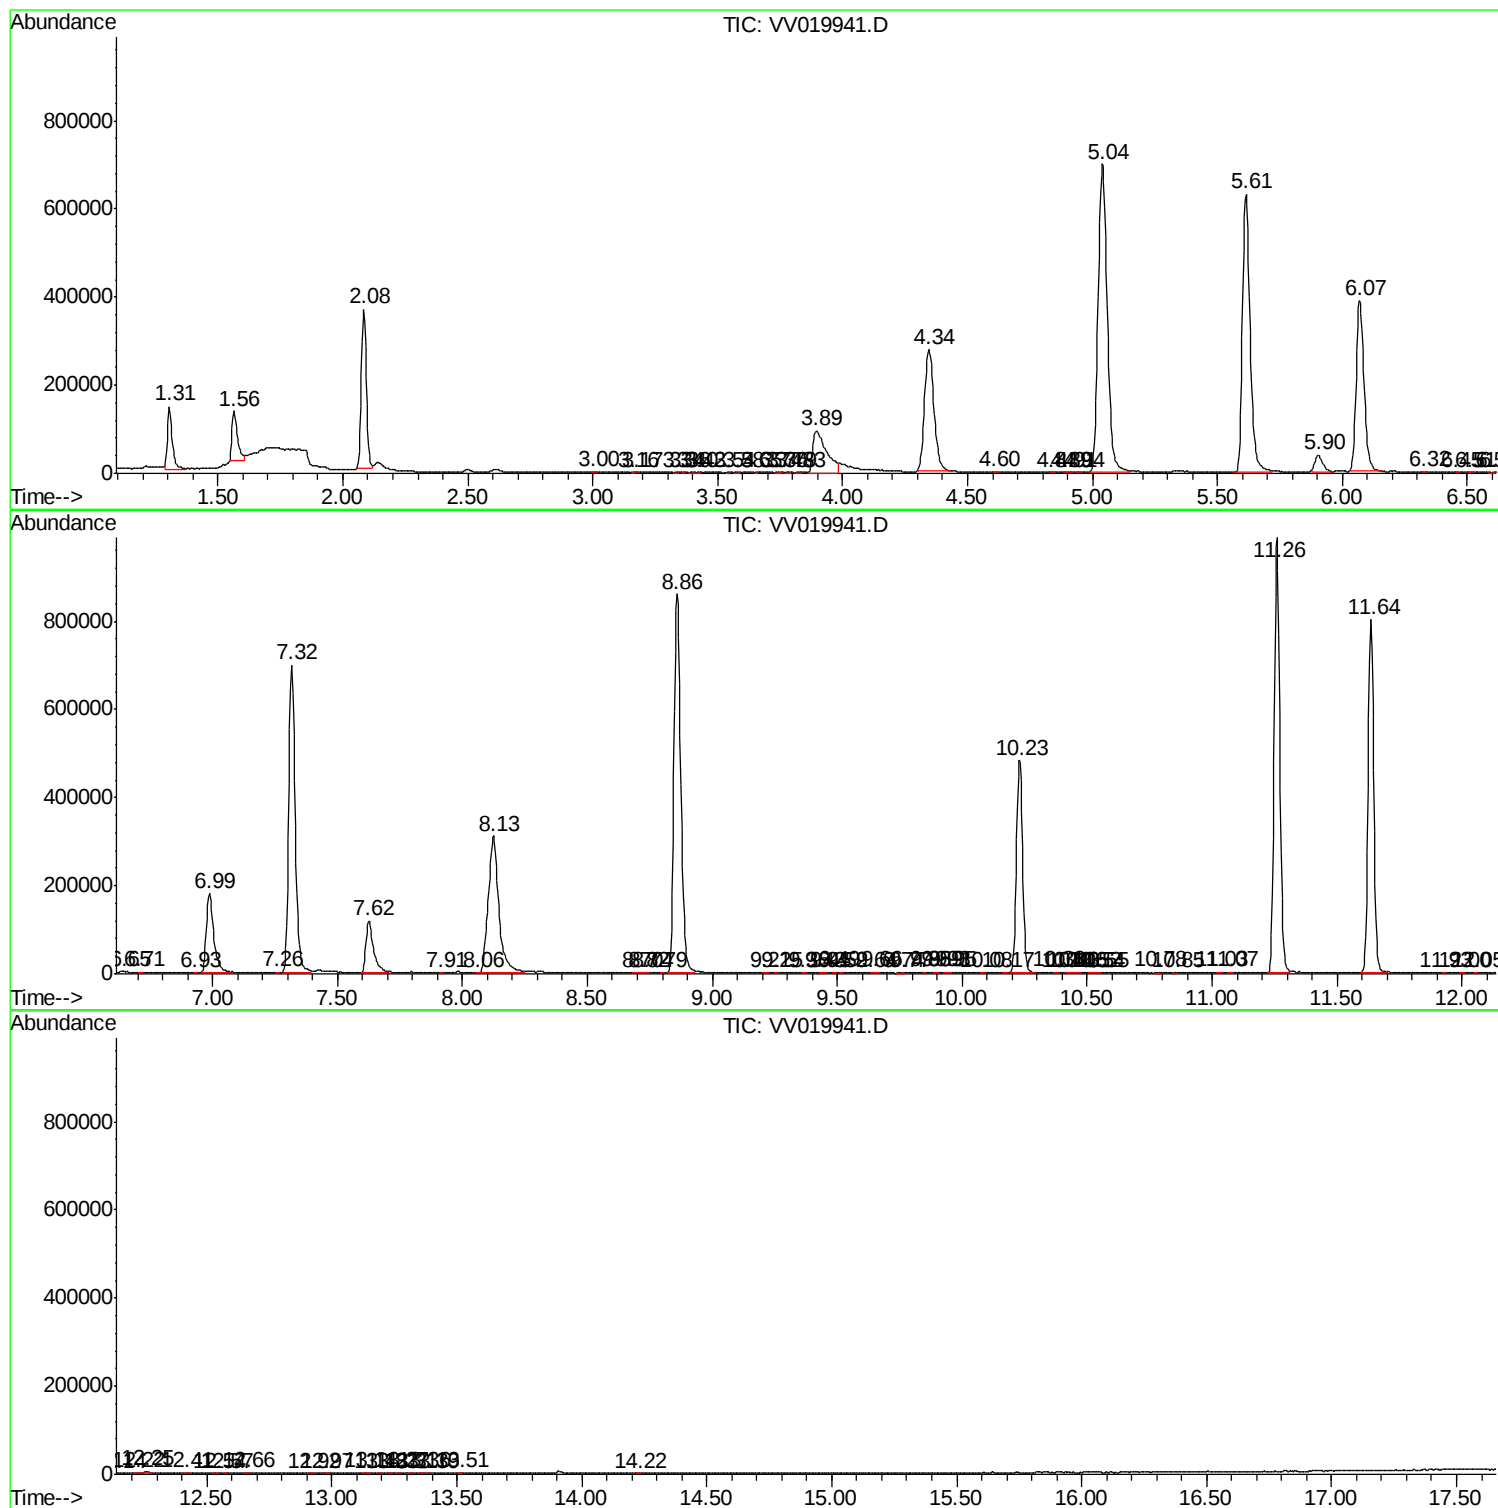

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010821\
Data File : VV019941.D
Acq On : 08 Jan 2021 12:35
Operator : SY/MD
Sample : M1053-01ME
Misc : 6.21g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BFN59ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010821\
Data File : VV019941.D
Acq On : 08 Jan 2021 12:35
Operator : SY/MD
Sample : M1053-01ME
Misc : 6.21g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BFN59ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc