

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019945.D
 Acq On : 08 Jan 2021 14:12
 Operator : SY/MD
 Sample : M1064-02 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	79	rVB	171967	178399	1.07%	0.569%
2	1.569	142	149	161	rVB	171885	192424	1.16%	0.614%
3	2.110	308	317	344	rVB	341165	539373	3.24%	1.722%
4	2.479	430	432	435	rBV3	1097	624	0.00%	0.002%
5	2.717	504	506	510	rBV4	605	519	0.00%	0.002%
6	2.753	514	517	518	rBV2	1238	612	0.00%	0.002%
7	2.810	533	535	537	rBV	763	329	0.00%	0.001%
8	2.827	537	540	541	rVV2	757	357	0.00%	0.001%
9	2.875	553	555	557	rBV3	458	282	0.00%	0.001%
10	2.974	584	586	591	rBV3	994	571	0.00%	0.002%
11	3.010	595	597	601	rBV3	484	459	0.00%	0.001%
12	3.097	622	624	627	rBV3	601	360	0.00%	0.001%
13	3.219	660	662	665	rBV3	814	468	0.00%	0.001%
14	3.248	669	671	674	rBV3	894	714	0.00%	0.002%
15	3.280	677	681	684	rBV5	1145	1034	0.01%	0.003%
16	3.296	684	686	691	rVB4	1257	829	0.00%	0.003%
17	3.318	691	693	696	rBV3	610	342	0.00%	0.001%
18	3.392	714	716	718	rBV3	668	347	0.00%	0.001%
19	3.463	734	738	741	rBV3	934	777	0.00%	0.002%
20	3.550	763	765	768	rBV2	437	271	0.00%	0.001%
21	3.563	768	769	773	rVB3	850	311	0.00%	0.001%
22	3.598	776	780	782	rBV4	590	510	0.00%	0.002%
23	3.666	798	801	802	rBV3	524	323	0.00%	0.001%
24	3.704	808	813	815	rBV3	768	708	0.00%	0.002%
25	3.717	815	817	819	rVB3	849	326	0.00%	0.001%
26	3.730	819	821	822	rBV3	643	276	0.00%	0.001%
27	3.769	828	833	839	rVV7	1498	1360	0.01%	0.004%
28	3.794	839	841	844	rVB2	625	296	0.00%	0.001%
29	3.855	858	860	861	rBV2	994	493	0.00%	0.002%
30	3.897	862	873	910	rVV	158447	514483	3.09%	1.642%
31	4.354	1000	1015	1039	rBV	282327	681337	4.10%	2.175%
32	4.659	1106	1110	1113	rBV5	1272	1004	0.01%	0.003%
33	4.891	1179	1182	1184	rBV3	826	577	0.00%	0.002%
34	4.926	1191	1193	1196	rBV2	795	521	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019945.D
 Acq On : 08 Jan 2021 14:12
 Operator : SY/MD
 Sample : M1064-02 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	4.939	1196	1197	1200	rVB	909	363	0.00%	0.001%
36	4.958	1200	1203	1204	rBV2	614	316	0.00%	0.001%
37	4.971	1204	1207	1208	rBV2	754	412	0.00%	0.001%
38	5.052	1215	1232	1263	rBV2	625460	1655763	9.96%	5.285%
39	5.543	1384	1385	1388	rBV2	804	393	0.00%	0.001%
40	5.621	1396	1409	1442	rBV	604610	1225549	7.37%	3.912%
41	5.920	1488	1502	1524	rBV2	454167	922123	5.55%	2.943%
42	6.074	1539	1550	1572	rVB	382973	769927	4.63%	2.458%
43	6.444	1661	1665	1671	rBV6	1018	1017	0.01%	0.003%
44	6.479	1673	1676	1679	rVB4	1279	772	0.00%	0.002%
45	6.515	1679	1687	1693	rBV9	1913	2287	0.01%	0.007%
46	6.537	1693	1694	1698	rVB2	811	435	0.00%	0.001%
47	6.560	1698	1701	1702	rBV2	670	408	0.00%	0.001%
48	6.630	1714	1723	1725	rBV6	2065	2580	0.02%	0.008%
49	6.724	1750	1752	1754	rBV3	922	325	0.00%	0.001%
50	6.868	1794	1797	1801	rBV4	1065	617	0.00%	0.002%
51	6.920	1808	1813	1817	rBV6	946	1000	0.01%	0.003%
52	6.990	1824	1835	1858	rBV	194092	356567	2.14%	1.138%
53	7.322	1925	1938	1961	rBV	669692	1173060	7.05%	3.744%
54	7.627	2024	2033	2060	rVB2	131458	232589	1.40%	0.742%
55	7.862	2103	2106	2107	rBV3	673	365	0.00%	0.001%
56	7.897	2114	2117	2120	rBV4	1074	932	0.01%	0.003%
57	7.981	2127	2143	2168	rBV	10067773	16627992	100.00%	53.076%
58	8.093	2169	2178	2209	rVB2	532725	1012617	6.09%	3.232%
59	8.627	2341	2344	2346	rBV3	1233	878	0.01%	0.003%
60	8.733	2374	2377	2380	rBV3	952	493	0.00%	0.002%
61	8.855	2404	2415	2448	rBV	932356	1533038	9.22%	4.893%
62	9.280	2545	2547	2554	rVB6	1173	1153	0.01%	0.004%
63	9.312	2554	2557	2562	rBV3	1302	977	0.01%	0.003%
64	9.479	2607	2609	2611	rBV2	530	318	0.00%	0.001%
65	9.508	2615	2618	2620	rBV3	1216	748	0.00%	0.002%
66	9.646	2658	2661	2663	rBV2	1354	614	0.00%	0.002%
67	9.749	2691	2693	2696	rBV2	719	426	0.00%	0.001%
68	9.775	2699	2701	2704	rBV4	1055	803	0.00%	0.003%
69	10.035	2779	2782	2790	rBV8	1226	1304	0.01%	0.004%
70	10.067	2790	2792	2794	rBV2	687	369	0.00%	0.001%
71	10.222	2828	2840	2859	rBV	560506	873539	5.25%	2.788%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019945.D
 Acq On : 08 Jan 2021 14:12
 Operator : SY/MD
 Sample : M1064-02 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.331	2873	2874	2877	rBV2	806	502	0.00%	0.002%
73	10.360	2881	2883	2886	rBV3	928	678	0.00%	0.002%
74	10.418	2897	2901	2902	rBV3	543	295	0.00%	0.001%
75	10.575	2948	2950	2951	rBV2	741	390	0.00%	0.001%
76	10.624	2963	2965	2969	rBV2	933	465	0.00%	0.001%
77	10.643	2969	2971	2973	rBV3	707	309	0.00%	0.001%
78	10.701	2983	2989	2991	rBV4	1087	987	0.01%	0.003%
79	10.823	3025	3027	3029	rBV2	920	449	0.00%	0.001%
80	10.926	3052	3059	3066	rBV8	1903	3453	0.02%	0.011%
81	11.006	3083	3084	3086	rBV2	799	393	0.00%	0.001%
82	11.090	3108	3110	3117	rVB3	911	688	0.00%	0.002%
83	11.190	3139	3141	3145	rBV3	757	550	0.00%	0.002%
84	11.257	3150	3162	3188	rBV	968680	1501977	9.03%	4.794%
85	11.489	3231	3234	3237	rBV4	719	525	0.00%	0.002%
86	11.633	3265	3279	3298	rBV	814023	1283102	7.72%	4.096%
87	11.916	3363	3367	3368	rBV4	611	444	0.00%	0.001%
88	11.945	3374	3376	3378	rBV2	707	396	0.00%	0.001%
89	12.125	3429	3432	3434	rBV3	1005	525	0.00%	0.002%
90	12.379	3509	3511	3515	rBV3	1016	790	0.00%	0.003%
91	12.974	3694	3696	3701	rVB3	791	627	0.00%	0.002%
92	13.000	3701	3704	3705	rBV2	865	502	0.00%	0.002%
93	13.206	3766	3768	3771	rBV2	834	581	0.00%	0.002%
94	13.283	3790	3792	3796	rBV4	1128	656	0.00%	0.002%
95	13.373	3815	3820	3822	rBV4	1113	987	0.01%	0.003%
96	13.437	3838	3840	3844	rBV3	887	683	0.00%	0.002%
97	13.537	3869	3871	3873	rBV3	952	514	0.00%	0.002%
98	13.849	3965	3968	3972	rBV3	1313	1218	0.01%	0.004%
99	14.337	4117	4120	4121	rBV2	1435	675	0.00%	0.002%
100	14.488	4165	4167	4170	rVB3	1180	477	0.00%	0.002%


Sum of corrected areas: 31328523

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010821\
Data File : VV019945.D
Acq On : 08 Jan 2021 14:12
Operator : SY/MD
Sample : M1064-02 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

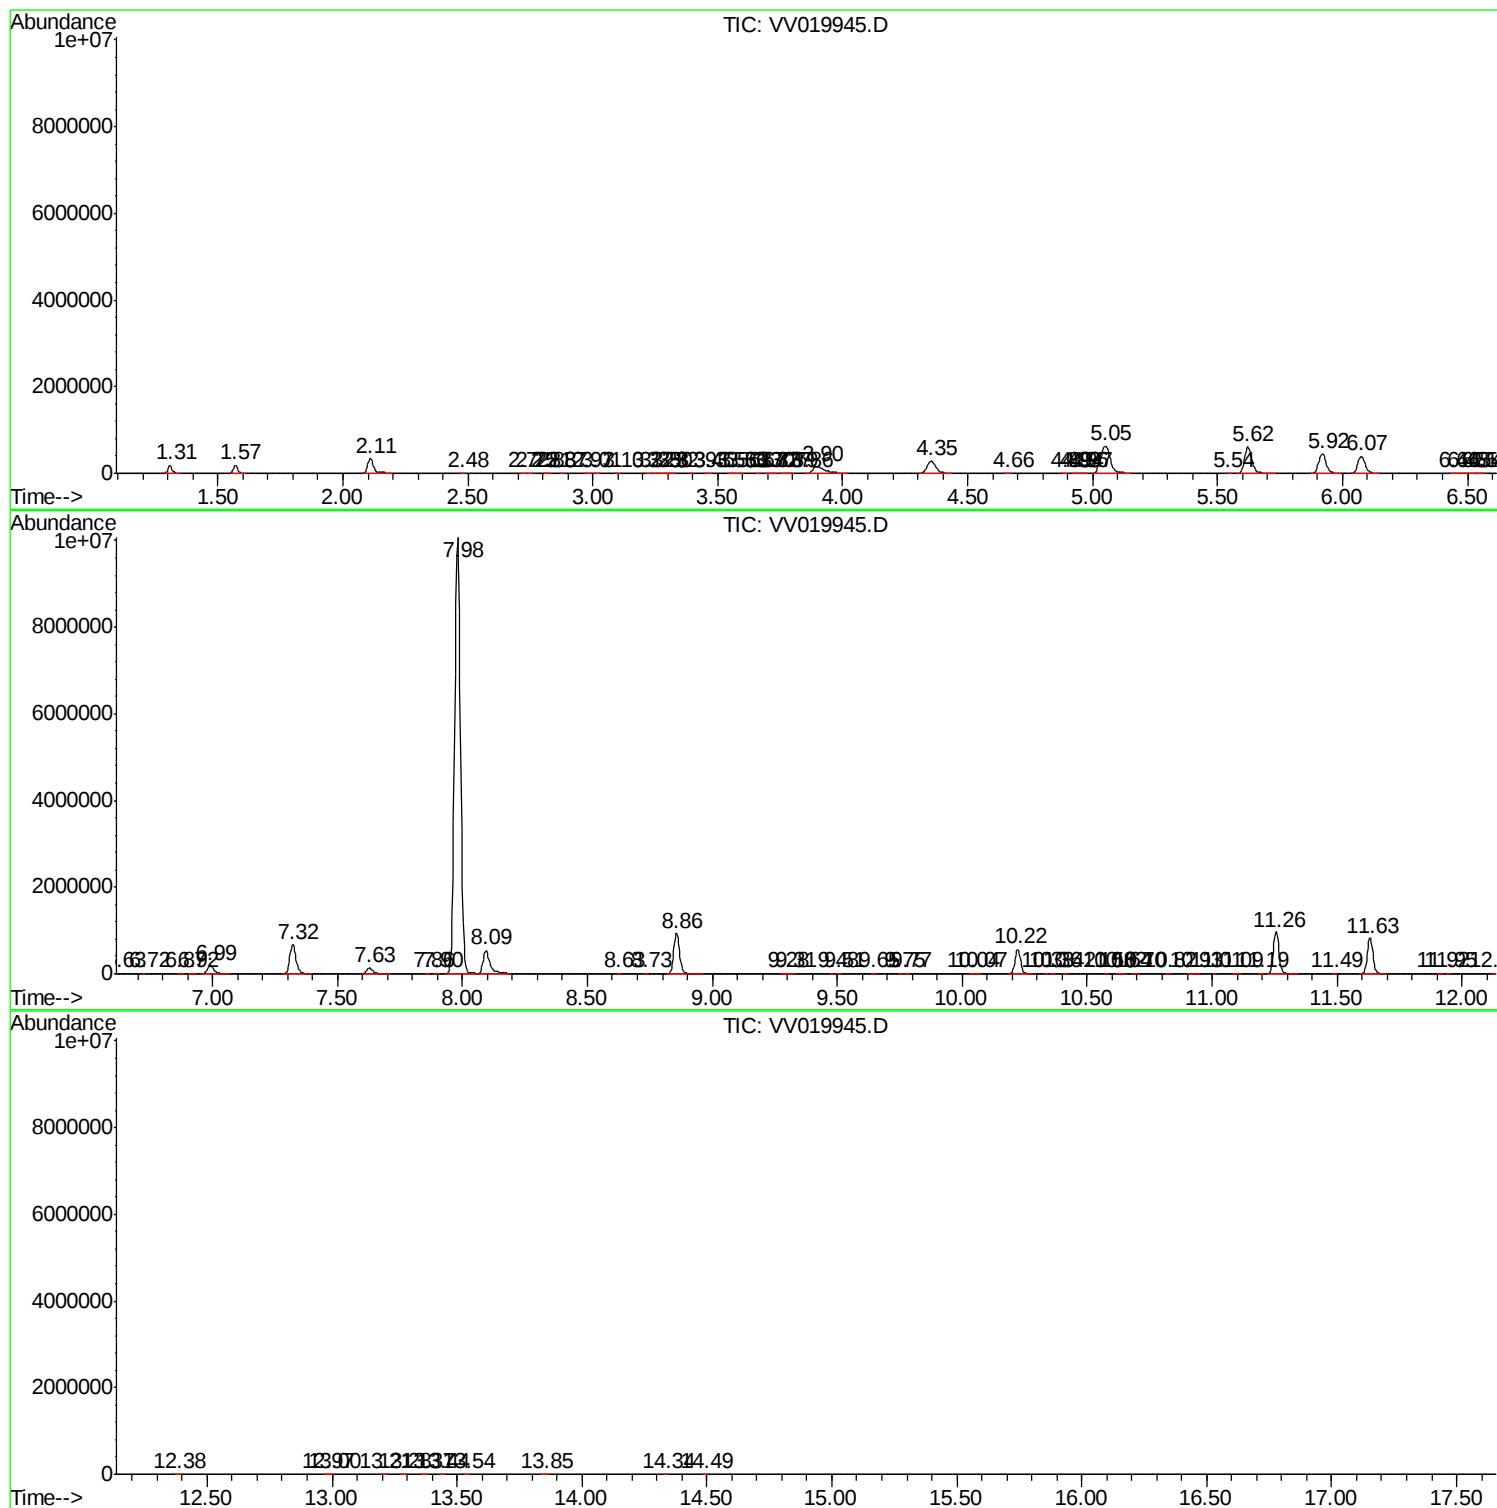

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019945.D
Acq On : 08 Jan 2021 14:12
Operator : SY/MD
Sample : M1064-02 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019945.D
Acq On : 08 Jan 2021 14:12
Operator : SY/MD
Sample : M1064-02 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc