

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019947.D
 Acq On : 08 Jan 2021 14:59
 Operator : SY/MD
 Sample : M1064-04 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.306	61	67	80	rVB	170220	167090	1.82%	0.741%
2	1.566	142	148	159	rVB	164481	177528	1.93%	0.787%
3	2.106	307	316	343	rVB	312349	498838	5.44%	2.211%
4	2.280	368	370	371	rBV2	1105	456	0.00%	0.002%
5	2.646	482	484	486	rBV	1037	506	0.01%	0.002%
6	2.704	500	502	505	rBV3	1102	688	0.01%	0.003%
7	2.830	538	541	544	rBV3	684	625	0.01%	0.003%
8	2.846	544	546	547	rBV2	689	265	0.00%	0.001%
9	2.878	553	556	559	rBV3	660	439	0.00%	0.002%
10	2.933	568	573	575	rBV3	990	975	0.01%	0.004%
11	3.016	596	599	602	rBV4	1475	1139	0.01%	0.005%
12	3.029	602	603	606	rVV3	773	413	0.00%	0.002%
13	3.161	642	644	646	rBV3	872	524	0.01%	0.002%
14	3.209	655	659	661	rBV3	836	651	0.01%	0.003%
15	3.219	661	662	664	rBV	502	197	0.00%	0.001%
16	3.270	675	678	680	rBV3	656	451	0.00%	0.002%
17	3.351	700	703	705	rBV4	883	607	0.01%	0.003%
18	3.405	718	720	721	rBV2	451	119	0.00%	0.001%
19	3.431	725	728	729	rBV2	593	322	0.00%	0.001%
20	3.460	736	737	740	rVB	452	178	0.00%	0.001%
21	3.476	740	742	744	rBV2	562	315	0.00%	0.001%
22	3.630	785	790	791	rBV3	496	433	0.00%	0.002%
23	3.656	796	798	803	rVV4	859	716	0.01%	0.003%
24	3.714	814	816	817	rBV2	750	340	0.00%	0.002%
25	3.765	829	832	836	rBV5	1157	992	0.01%	0.004%
26	3.891	857	871	907	rBV2	157014	481476	5.25%	2.134%
27	4.351	1000	1014	1037	rBV2	267080	646278	7.04%	2.864%
28	4.788	1146	1150	1151	rBV4	947	540	0.01%	0.002%
29	4.826	1160	1162	1163	rBV	1245	411	0.00%	0.002%
30	4.933	1194	1195	1197	rBV2	539	202	0.00%	0.001%
31	4.965	1202	1205	1207	rBV3	549	377	0.00%	0.002%
32	4.978	1207	1209	1212	rBV2	595	275	0.00%	0.001%
33	5.048	1212	1231	1258	rBV2	591593	1548838	16.88%	6.864%
34	5.328	1314	1318	1320	rBV4	1097	928	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019947.D
 Acq On : 08 Jan 2021 14:59
 Operator : SY/MD
 Sample : M1064-04 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	5.396	1336	1339	1340	rBV2	1396	797	0.01%	0.004%
36	5.469	1360	1362	1363	rBV2	749	294	0.00%	0.001%
37	5.492	1366	1369	1372	rVV3	1760	1011	0.01%	0.004%
38	5.537	1381	1383	1387	rBV5	978	694	0.01%	0.003%
39	5.621	1396	1409	1436	rBV	567035	1131145	12.33%	5.013%
40	5.916	1488	1501	1522	rBV3	268563	563139	6.14%	2.496%
41	6.074	1538	1550	1578	rVB	371465	746308	8.13%	3.307%
42	6.441	1662	1664	1668	rBV4	921	647	0.01%	0.003%
43	6.479	1674	1676	1678	rVB2	906	320	0.00%	0.001%
44	6.733	1753	1755	1757	rBV2	762	329	0.00%	0.001%
45	6.836	1783	1787	1788	rBV3	1060	784	0.01%	0.003%
46	6.900	1805	1807	1809	rBV3	959	433	0.00%	0.002%
47	6.945	1818	1821	1822	rVB3	560	278	0.00%	0.001%
48	6.990	1822	1835	1852	rBV	179616	333216	3.63%	1.477%
49	7.322	1926	1938	1964	rBV	628861	1097034	11.96%	4.862%
50	7.627	2023	2033	2057	rBV2	126348	221853	2.42%	0.983%
51	7.981	2127	2143	2167	rBV	5502663	9174751	100.00%	40.661%
52	8.093	2169	2178	2222	rVB2	478432	959421	10.46%	4.252%
53	8.855	2404	2415	2442	rBV	859507	1414474	15.42%	6.269%
54	9.485	2609	2611	2613	rBV2	496	254	0.00%	0.001%
55	9.547	2626	2630	2634	rBV4	734	485	0.01%	0.002%
56	9.682	2667	2672	2675	rBV6	959	775	0.01%	0.003%
57	9.694	2675	2676	2678	rBV2	542	282	0.00%	0.001%
58	9.736	2687	2689	2691	rBV2	860	450	0.00%	0.002%
59	9.797	2706	2708	2709	rBV2	679	332	0.00%	0.001%
60	9.939	2748	2752	2753	rBV2	424	245	0.00%	0.001%
61	9.948	2753	2755	2757	rVB3	754	313	0.00%	0.001%
62	9.977	2763	2764	2766	rBV2	723	330	0.00%	0.001%
63	10.051	2783	2787	2789	rBV3	840	582	0.01%	0.003%
64	10.093	2798	2800	2806	rVB5	1239	706	0.01%	0.003%
65	10.222	2828	2840	2862	rVB	522030	811580	8.85%	3.597%
66	10.395	2893	2894	2897	rBV3	1144	597	0.01%	0.003%
67	10.453	2910	2912	2913	rBV2	675	263	0.00%	0.001%
68	10.543	2938	2940	2943	rBV2	1079	551	0.01%	0.002%
69	10.582	2950	2952	2956	rBV2	830	412	0.00%	0.002%
70	10.601	2956	2958	2959	rBV2	605	231	0.00%	0.001%
71	10.627	2963	2966	2969	rBV4	1082	926	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019947.D
 Acq On : 08 Jan 2021 14:59
 Operator : SY/MD
 Sample : M1064-04 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.749	3001	3004	3006	rBV3	942	541	0.01%	0.002%
73	10.810	3021	3023	3027	rBV2	854	530	0.01%	0.002%
74	10.971	3071	3073	3075	rBV2	661	311	0.00%	0.001%
75	11.016	3085	3087	3089	rVB3	609	184	0.00%	0.001%
76	11.061	3099	3101	3102	rBV	503	234	0.00%	0.001%
77	11.151	3127	3129	3131	rBV2	605	314	0.00%	0.001%
78	11.254	3150	3161	3181	rBV	870002	1364716	14.87%	6.048%
79	11.527	3242	3246	3247	rBV3	688	426	0.00%	0.002%
80	11.630	3266	3278	3296	rBV	747856	1191542	12.99%	5.281%
81	12.064	3411	3413	3416	rBV3	678	389	0.00%	0.002%
82	12.135	3432	3435	3442	rBV5	927	1059	0.01%	0.005%
83	12.553	3563	3565	3568	rBV3	849	596	0.01%	0.003%
84	12.723	3617	3618	3619	rBV3	1093	358	0.00%	0.002%
85	13.206	3766	3768	3769	rBV2	710	287	0.00%	0.001%
86	13.379	3819	3822	3823	rBV2	992	587	0.01%	0.003%
87	13.492	3854	3857	3858	rBV2	1060	619	0.01%	0.003%
88	13.572	3880	3882	3887	rBV3	1160	1143	0.01%	0.005%


Sum of corrected areas: 22564210

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010821\
Data File : VV019947.D
Acq On : 08 Jan 2021 14:59
Operator : SY/MD
Sample : M1064-04 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

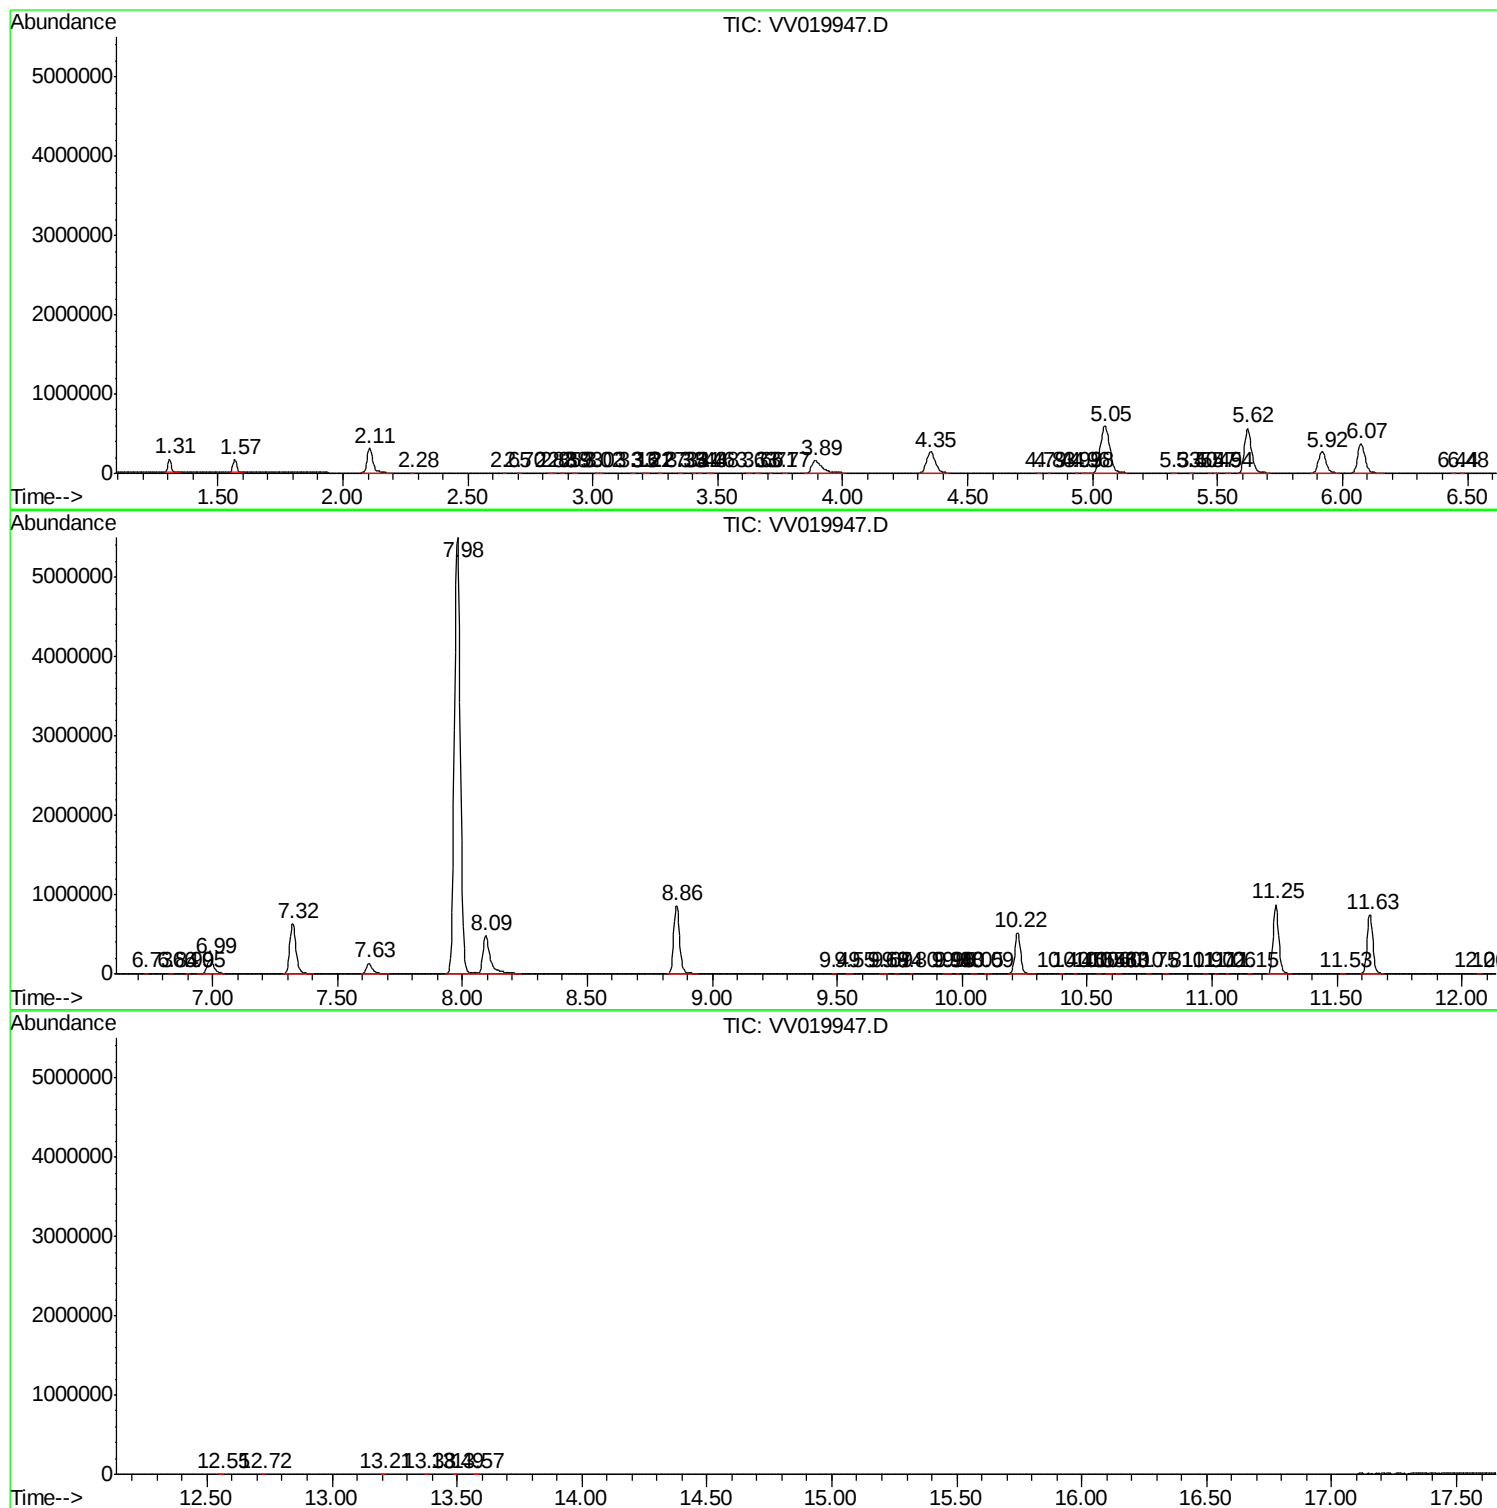

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019947.D
Acq On : 08 Jan 2021 14:59
Operator : SY/MD
Sample : M1064-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010821\
Data File : VV019947.D
Acq On : 08 Jan 2021 14:59
Operator : SY/MD
Sample : M1064-04 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4X5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc