

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019950.D
 Acq On : 08 Jan 2021 16:24
 Operator : SY/MD
 Sample : M1016-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	81	rVB	170753	170170	10.85%	1.302%
2	1.569	142	149	162	rVB	174178	197135	12.56%	1.508%
3	2.110	308	317	345	rVB	323294	517269	32.97%	3.958%
4	2.630	477	479	483	rBV5	851	899	0.06%	0.007%
5	2.945	573	577	578	rBV4	785	473	0.03%	0.004%
6	2.978	585	587	590	rVB4	761	457	0.03%	0.003%
7	3.045	595	608	622	rBV4	12344	28046	1.79%	0.215%
8	3.151	637	641	645	rBV4	848	738	0.05%	0.006%
9	3.212	656	660	664	rBV6	712	580	0.04%	0.004%
10	3.370	705	709	711	rBV5	998	655	0.04%	0.005%
11	3.428	721	727	728	rBV6	684	556	0.04%	0.004%
12	3.495	744	748	749	rVV3	695	453	0.03%	0.003%
13	3.592	775	778	780	rBV2	655	410	0.03%	0.003%
14	3.640	790	793	796	rBV4	786	522	0.03%	0.004%
15	3.682	800	806	808	rBV6	977	730	0.05%	0.006%
16	3.724	817	819	821	rVV3	1260	778	0.05%	0.006%
17	3.769	821	833	849	rVB4	7293	20245	1.29%	0.155%
18	3.884	856	869	902	rBV	149218	426102	27.16%	3.260%
19	4.354	1001	1015	1042	rVB	268518	657345	41.90%	5.029%
20	4.830	1158	1163	1167	rVB7	1223	1259	0.08%	0.010%
21	4.855	1167	1171	1174	rBV5	1370	833	0.05%	0.006%
22	4.871	1174	1176	1178	rBV3	820	425	0.03%	0.003%
23	4.961	1200	1204	1208	rBV5	895	1017	0.06%	0.008%
24	5.051	1214	1232	1260	rBV2	601617	1568986	100.00%	12.004%
25	5.373	1331	1332	1335	rBV3	978	505	0.03%	0.004%
26	5.498	1368	1371	1373	rBV4	1065	780	0.05%	0.006%
27	5.621	1396	1409	1431	rBV	577853	1155234	73.63%	8.839%
28	5.910	1489	1499	1517	rBV2	50155	102475	6.53%	0.784%
29	6.074	1537	1550	1573	rBV	373065	761233	48.52%	5.824%
30	6.325	1625	1628	1631	rBV3	854	710	0.05%	0.005%
31	6.392	1647	1649	1651	rBV3	943	607	0.04%	0.005%
32	6.524	1688	1690	1695	rBV5	745	711	0.05%	0.005%
33	6.592	1708	1711	1714	rVB4	909	571	0.04%	0.004%
34	6.633	1715	1724	1728	rBV8	2176	2935	0.19%	0.022%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019950.D
 Acq On : 08 Jan 2021 16:24
 Operator : SY/MD
 Sample : M1016-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	6.817	1776	1781	1783	rBV5	951	823	0.05%	0.006%
36	6.868	1794	1797	1798	rBV2	731	490	0.03%	0.004%
37	6.990	1824	1835	1855	rBV	182550	337164	21.49%	2.580%
38	7.322	1926	1938	1959	rBV	643166	1118414	71.28%	8.557%
39	7.582	2016	2019	2021	rBV3	1073	794	0.05%	0.006%
40	7.627	2023	2033	2055	rVV	128217	224747	14.32%	1.720%
41	7.865	2103	2107	2109	rBV4	1169	919	0.06%	0.007%
42	7.913	2119	2122	2124	rBV2	780	498	0.03%	0.004%
43	7.945	2128	2132	2135	rBV4	1810	1672	0.11%	0.013%
44	8.093	2168	2178	2215	rVV2	421238	883783	56.33%	6.762%
45	8.511	2304	2308	2313	rBV7	1408	1153	0.07%	0.009%
46	8.637	2345	2347	2349	rBV3	1005	425	0.03%	0.003%
47	8.691	2360	2364	2369	rVB6	1590	1428	0.09%	0.011%
48	8.762	2382	2386	2389	rBV4	1071	855	0.05%	0.007%
49	8.858	2402	2416	2443	rBV	893468	1457740	92.91%	11.153%
50	9.071	2480	2482	2485	rBV2	881	418	0.03%	0.003%
51	9.141	2500	2504	2506	rBV3	1840	1344	0.09%	0.010%
52	9.183	2515	2517	2523	rBV5	763	907	0.06%	0.007%
53	9.292	2548	2551	2556	rBV6	1167	1269	0.08%	0.010%
54	9.360	2570	2572	2576	rBV2	781	417	0.03%	0.003%
55	9.463	2603	2604	2609	rVB3	819	553	0.04%	0.004%
56	9.495	2609	2614	2617	rBV6	974	1164	0.07%	0.009%
57	9.524	2620	2623	2626	rBV2	977	704	0.04%	0.005%
58	9.540	2626	2628	2631	rBV4	940	708	0.05%	0.005%
59	9.704	2677	2679	2682	rBV3	852	474	0.03%	0.004%
60	9.881	2730	2734	2738	rBV3	869	792	0.05%	0.006%
61	9.968	2758	2761	2763	rBV4	932	452	0.03%	0.003%
62	10.016	2773	2776	2780	rVB5	1160	918	0.06%	0.007%
63	10.083	2794	2797	2799	rBV3	720	431	0.03%	0.003%
64	10.116	2804	2807	2811	rVB4	963	616	0.04%	0.005%
65	10.141	2811	2815	2817	rBV4	1046	837	0.05%	0.006%
66	10.154	2817	2819	2822	rVB3	933	487	0.03%	0.004%
67	10.222	2829	2840	2862	rVB	482540	757442	48.28%	5.795%
68	10.389	2884	2892	2900	rVV6	6205	10790	0.69%	0.083%
69	10.669	2975	2979	2982	rBV5	1098	817	0.05%	0.006%
70	10.730	2994	2998	3002	rVV4	1161	686	0.04%	0.005%
71	10.923	3051	3058	3068	rBV8	1776	2848	0.18%	0.022%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019950.D
 Acq On : 08 Jan 2021 16:24
 Operator : SY/MD
 Sample : M1016-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.990	3077	3079	3082	rBV3	760	454	0.03%	0.003%
73	11.071	3102	3104	3110	rBV5	791	673	0.04%	0.005%
74	11.180	3132	3138	3143	rVB7	1462	1493	0.10%	0.011%
75	11.254	3150	3161	3181	rBV	880355	1383928	88.21%	10.588%
76	11.460	3222	3225	3228	rBV5	1319	1005	0.06%	0.008%
77	11.508	3233	3240	3244	rBV6	1650	2109	0.13%	0.016%
78	11.540	3246	3250	3251	rBV2	1154	896	0.06%	0.007%
79	11.630	3266	3278	3301	rBV	771262	1223874	78.00%	9.364%
80	11.865	3348	3351	3353	rBV3	735	484	0.03%	0.004%
81	11.929	3369	3371	3374	rBV3	1389	951	0.06%	0.007%
82	12.099	3420	3424	3425	rBV3	1016	709	0.05%	0.005%
83	12.144	3432	3438	3441	rVB6	783	774	0.05%	0.006%
84	12.238	3465	3467	3468	rBV3	1370	564	0.04%	0.004%
85	12.305	3486	3488	3491	rBV3	728	454	0.03%	0.003%
86	12.366	3498	3507	3511	rBV10	3115	4216	0.27%	0.032%
87	12.521	3552	3555	3556	rBV2	878	505	0.03%	0.004%
88	12.595	3574	3578	3583	rBV4	715	612	0.04%	0.005%
89	12.688	3605	3607	3612	rVB3	1333	898	0.06%	0.007%
90	12.884	3666	3668	3671	rVV3	699	414	0.03%	0.003%
91	12.910	3674	3676	3680	rBV2	1148	740	0.05%	0.006%
92	12.929	3680	3682	3686	rBV3	709	488	0.03%	0.004%
93	13.167	3753	3756	3760	rBV3	1447	1279	0.08%	0.010%
94	13.617	3894	3896	3897	rBV	1158	447	0.03%	0.003%
95	13.759	3937	3940	3943	rBV5	1274	783	0.05%	0.006%
96	13.913	3985	3988	3991	rVV3	1295	1019	0.06%	0.008%
97	13.932	3991	3994	3999	rVB6	1220	1145	0.07%	0.009%
98	14.189	4072	4074	4076	rBV2	720	428	0.03%	0.003%
99	14.247	4089	4092	4093	rBV2	768	490	0.03%	0.004%
100	14.742	4244	4246	4250	rBV5	904	648	0.04%	0.005%


Sum of corrected areas: 13070303

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010821\
Data File : VV019950.D
Acq On : 08 Jan 2021 16:24
Operator : SY/MD
Sample : M1016-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

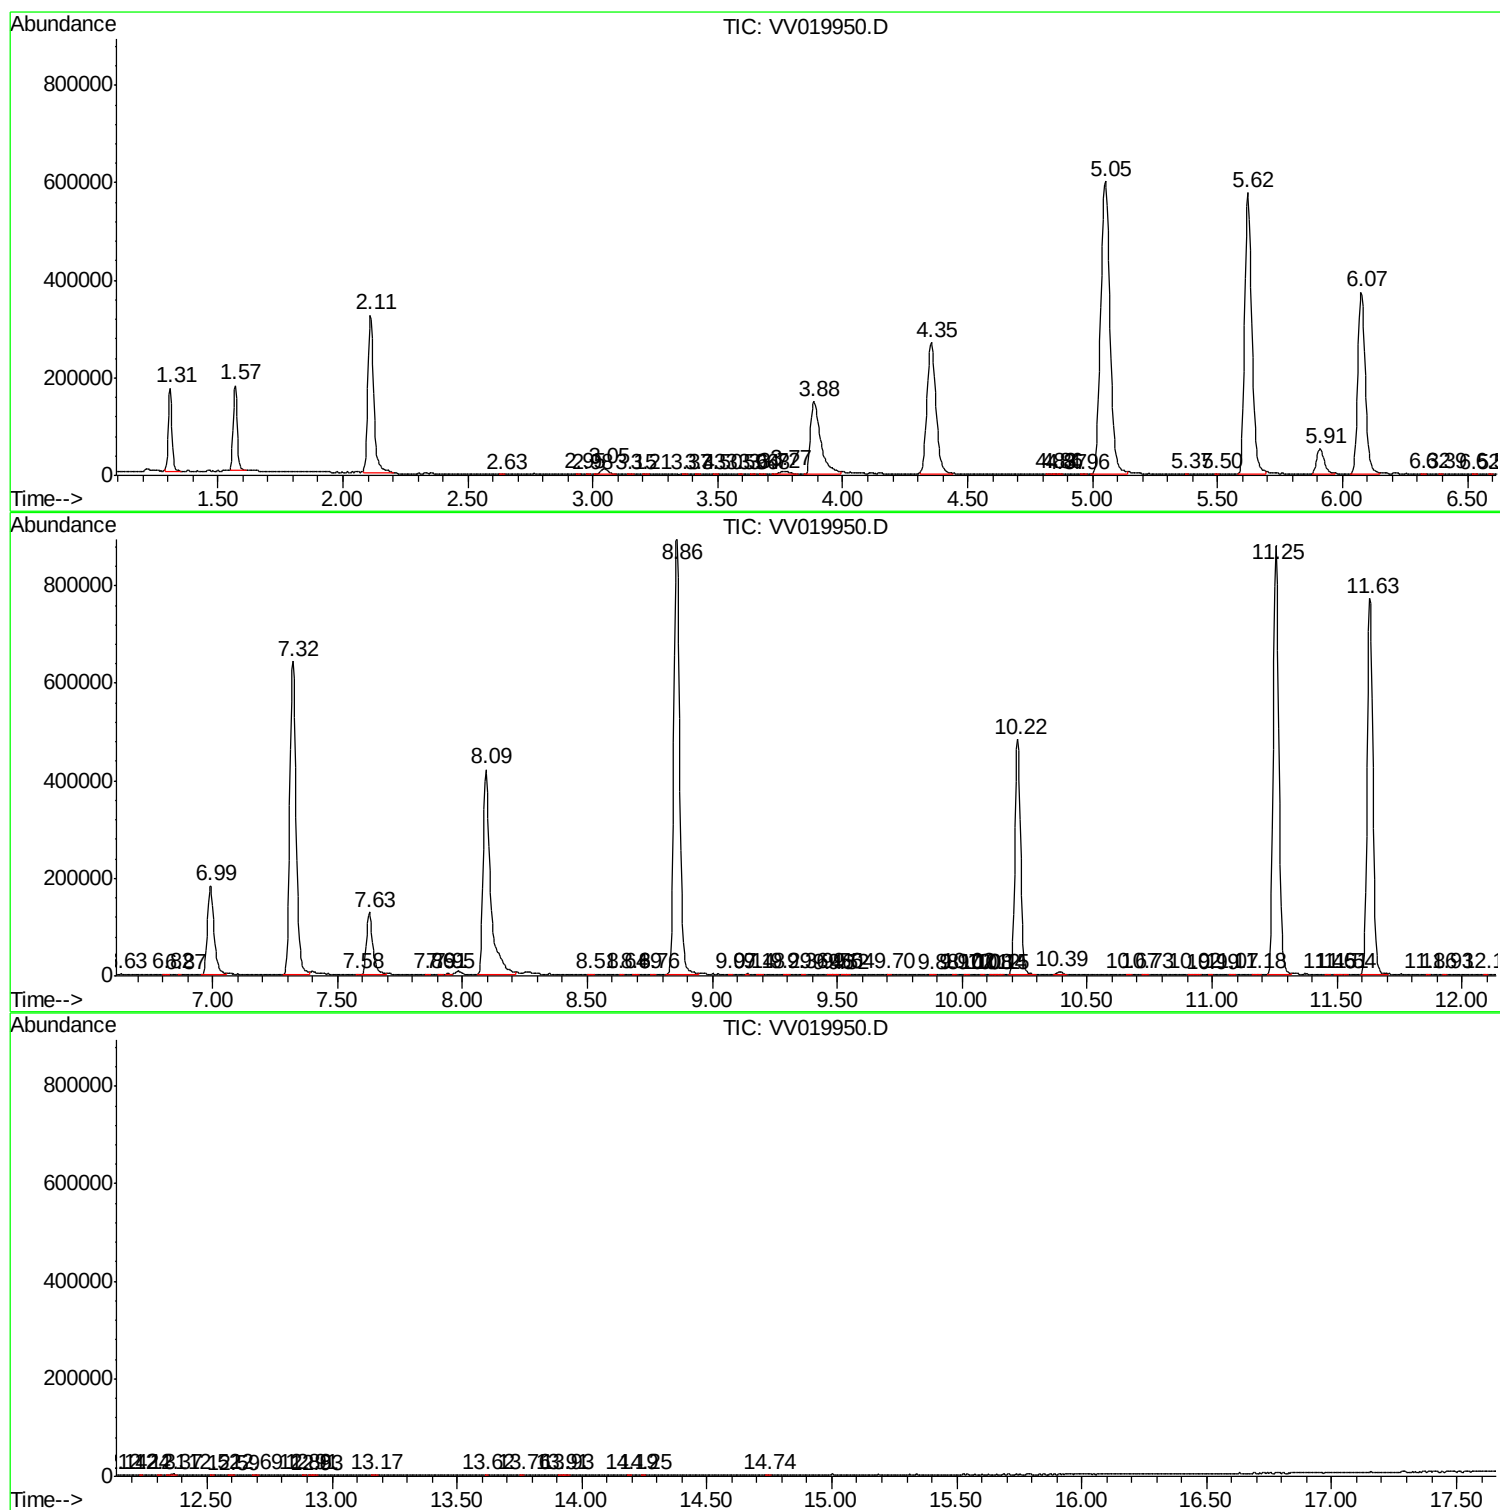

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010821\
Data File : VV019950.D
Acq On : 08 Jan 2021 16:24
Operator : SY/MD
Sample : M1016-13
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4T7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010821\
Data File : VV019950.D
Acq On : 08 Jan 2021 16:24
Operator : SY/MD
Sample : M1016-13
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4T7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc