

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019953.D
 Acq On : 08 Jan 2021 17:34
 Operator : SY/MD
 Sample : M1064-03DL 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	77	rVB	156218	155329	6.21%	1.001%
2	1.569	142	149	160	rBV	162621	181664	7.27%	1.171%
3	2.110	308	317	343	rVB2	299976	484028	19.36%	3.121%
4	2.428	413	416	418	rBV4	1237	708	0.03%	0.005%
5	2.553	453	455	456	rBV3	793	279	0.01%	0.002%
6	2.595	462	468	470	rBV4	1235	1289	0.05%	0.008%
7	2.733	508	511	514	rBV3	814	594	0.02%	0.004%
8	2.807	532	534	536	rVB2	964	362	0.01%	0.002%
9	2.823	536	539	543	rBV4	911	693	0.03%	0.004%
10	2.904	561	564	566	rBV4	702	495	0.02%	0.003%
11	2.946	575	577	579	rBV3	687	404	0.02%	0.003%
12	3.142	636	638	639	rBV3	786	301	0.01%	0.002%
13	3.167	644	646	648	rBV	708	444	0.02%	0.003%
14	3.200	652	656	660	rBV7	641	636	0.03%	0.004%
15	3.219	660	662	663	rBV	569	198	0.01%	0.001%
16	3.254	670	673	675	rBV2	920	574	0.02%	0.004%
17	3.286	681	683	685	rVB3	683	187	0.01%	0.001%
18	3.380	709	712	715	rBV3	625	487	0.02%	0.003%
19	3.415	719	723	725	rBV	524	378	0.02%	0.002%
20	3.460	730	737	742	rBV5	845	1160	0.05%	0.007%
21	3.483	742	744	747	rBV4	548	348	0.01%	0.002%
22	3.550	763	765	766	rBV2	922	386	0.02%	0.002%
23	3.614	784	785	787	rBV2	704	295	0.01%	0.002%
24	3.659	798	799	803	rVB3	601	324	0.01%	0.002%
25	3.692	804	809	812	rBV5	832	821	0.03%	0.005%
26	3.720	816	818	820	rBV2	674	380	0.02%	0.002%
27	3.753	825	828	831	rBV2	1013	756	0.03%	0.005%
28	3.827	849	851	854	rVB2	791	424	0.02%	0.003%
29	3.888	858	870	907	rBV	165823	488630	19.54%	3.150%
30	4.267	987	988	992	rBV3	906	635	0.03%	0.004%
31	4.354	1000	1015	1040	rBV	261478	640380	25.61%	4.129%
32	4.775	1142	1146	1147	rBV3	727	521	0.02%	0.003%
33	4.823	1159	1161	1165	rBV3	859	530	0.02%	0.003%
34	4.862	1171	1173	1176	rBV4	743	530	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019953.D
 Acq On : 08 Jan 2021 17:34
 Operator : SY/MD
 Sample : M1064-03DL 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	4.939	1190	1197	1200	rBV6	834	937	0.04%	0.006%
36	5.052	1215	1232	1262	rBV2	578281	1510158	60.40%	9.737%
37	5.383	1333	1335	1337	rBV3	670	283	0.01%	0.002%
38	5.437	1350	1352	1356	rBV3	1032	730	0.03%	0.005%
39	5.569	1391	1393	1394	rBV2	893	464	0.02%	0.003%
40	5.621	1394	1409	1438	rVV	582347	1178342	47.13%	7.597%
41	5.917	1489	1501	1518	rBV5	89914	203841	8.15%	1.314%
42	6.010	1528	1530	1532	rBV3	1303	462	0.02%	0.003%
43	6.074	1538	1550	1570	rBV	363761	734966	29.40%	4.739%
44	6.338	1629	1632	1635	rBV4	1227	930	0.04%	0.006%
45	6.412	1650	1655	1657	rBV5	1030	926	0.04%	0.006%
46	6.611	1713	1717	1718	rBV3	973	721	0.03%	0.005%
47	6.634	1718	1724	1727	rBV6	2288	2451	0.10%	0.016%
48	6.781	1767	1770	1773	rVB3	1404	831	0.03%	0.005%
49	6.798	1773	1775	1776	rBV2	700	275	0.01%	0.002%
50	6.843	1787	1789	1792	rBV3	768	253	0.01%	0.002%
51	6.990	1823	1835	1855	rBV	175261	326952	13.08%	2.108%
52	7.322	1926	1938	1960	rBV	595493	1051679	42.06%	6.781%
53	7.585	2018	2020	2022	rBV3	940	488	0.02%	0.003%
54	7.627	2023	2033	2051	rVV	123704	217535	8.70%	1.403%
55	7.981	2129	2143	2167	rBV	1487883	2500213	100.00%	16.120%
56	8.093	2168	2178	2209	rBV2	485939	940828	37.63%	6.066%
57	8.859	2403	2416	2436	rBV	892218	1464232	58.56%	9.441%
58	9.190	2517	2519	2520	rBV	862	412	0.02%	0.003%
59	9.495	2609	2614	2616	rBV3	1201	1066	0.04%	0.007%
60	9.617	2650	2652	2655	rVB2	832	349	0.01%	0.002%
61	9.794	2705	2707	2710	rBV4	772	562	0.02%	0.004%
62	9.823	2714	2716	2719	rVB3	786	369	0.01%	0.002%
63	9.836	2719	2720	2721	rBV	744	261	0.01%	0.002%
64	9.878	2732	2733	2736	rVB3	1017	390	0.02%	0.003%
65	10.093	2798	2800	2801	rBV2	827	276	0.01%	0.002%
66	10.138	2812	2814	2816	rBV3	577	321	0.01%	0.002%
67	10.222	2828	2840	2861	rBV	524189	820651	32.82%	5.291%
68	10.421	2900	2902	2906	rBV3	1014	702	0.03%	0.005%
69	10.473	2916	2918	2923	rVB3	942	630	0.03%	0.004%
70	10.505	2923	2928	2932	rBV5	1104	1215	0.05%	0.008%
71	10.666	2976	2978	2981	rBV3	827	611	0.02%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019953.D
 Acq On : 08 Jan 2021 17:34
 Operator : SY/MD
 Sample : M1064-03DL 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.730	2996	2998	3000	rBV2	952	366	0.01%	0.002%
73	10.756	3002	3006	3007	rBV3	1051	765	0.03%	0.005%
74	10.791	3012	3017	3019	rBV4	1109	796	0.03%	0.005%
75	10.804	3019	3021	3027	rVB5	729	540	0.02%	0.003%
76	10.965	3069	3071	3073	rBV2	944	348	0.01%	0.002%
77	10.977	3073	3075	3078	rVB3	799	408	0.02%	0.003%
78	11.109	3111	3116	3119	rVB5	1054	941	0.04%	0.006%
79	11.125	3119	3121	3124	rBV3	959	681	0.03%	0.004%
80	11.167	3131	3134	3135	rBV2	1275	746	0.03%	0.005%
81	11.257	3149	3162	3182	rBV	901239	1402120	56.08%	9.040%
82	11.630	3266	3278	3298	rBV	737485	1161584	46.46%	7.489%
83	11.926	3368	3370	3373	rBV3	806	394	0.02%	0.003%
84	11.987	3388	3389	3393	rVB3	752	361	0.01%	0.002%
85	12.006	3393	3395	3398	rVB2	591	233	0.01%	0.002%
86	12.067	3412	3414	3419	rVB4	935	684	0.03%	0.004%
87	12.338	3496	3498	3499	rVB2	743	179	0.01%	0.001%
88	12.395	3510	3516	3521	rBV6	1330	1785	0.07%	0.012%
89	12.460	3534	3536	3538	rBV2	794	408	0.02%	0.003%
90	12.624	3584	3587	3589	rBV3	909	602	0.02%	0.004%
91	12.756	3626	3628	3631	rBV4	1079	662	0.03%	0.004%
92	12.817	3645	3647	3648	rBV2	777	319	0.01%	0.002%
93	12.874	3663	3665	3669	rVB4	765	316	0.01%	0.002%
94	12.981	3697	3698	3700	rBV2	729	234	0.01%	0.002%
95	13.800	3951	3953	3956	rBV3	852	290	0.01%	0.002%
96	13.945	3996	3998	4002	rBV4	799	327	0.01%	0.002%
97	14.337	4118	4120	4122	rBV3	1176	765	0.03%	0.005%
98	14.437	4149	4151	4155	rBV2	1097	645	0.03%	0.004%
99	14.656	4217	4219	4221	rBV3	1017	291	0.01%	0.002%
100	14.730	4241	4242	4245	rBV2	991	587	0.02%	0.004%


Sum of corrected areas: 15509859

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010821\
Data File : VV019953.D
Acq On : 08 Jan 2021 17:34
Operator : SY/MD
Sample : M1064-03DL 250X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

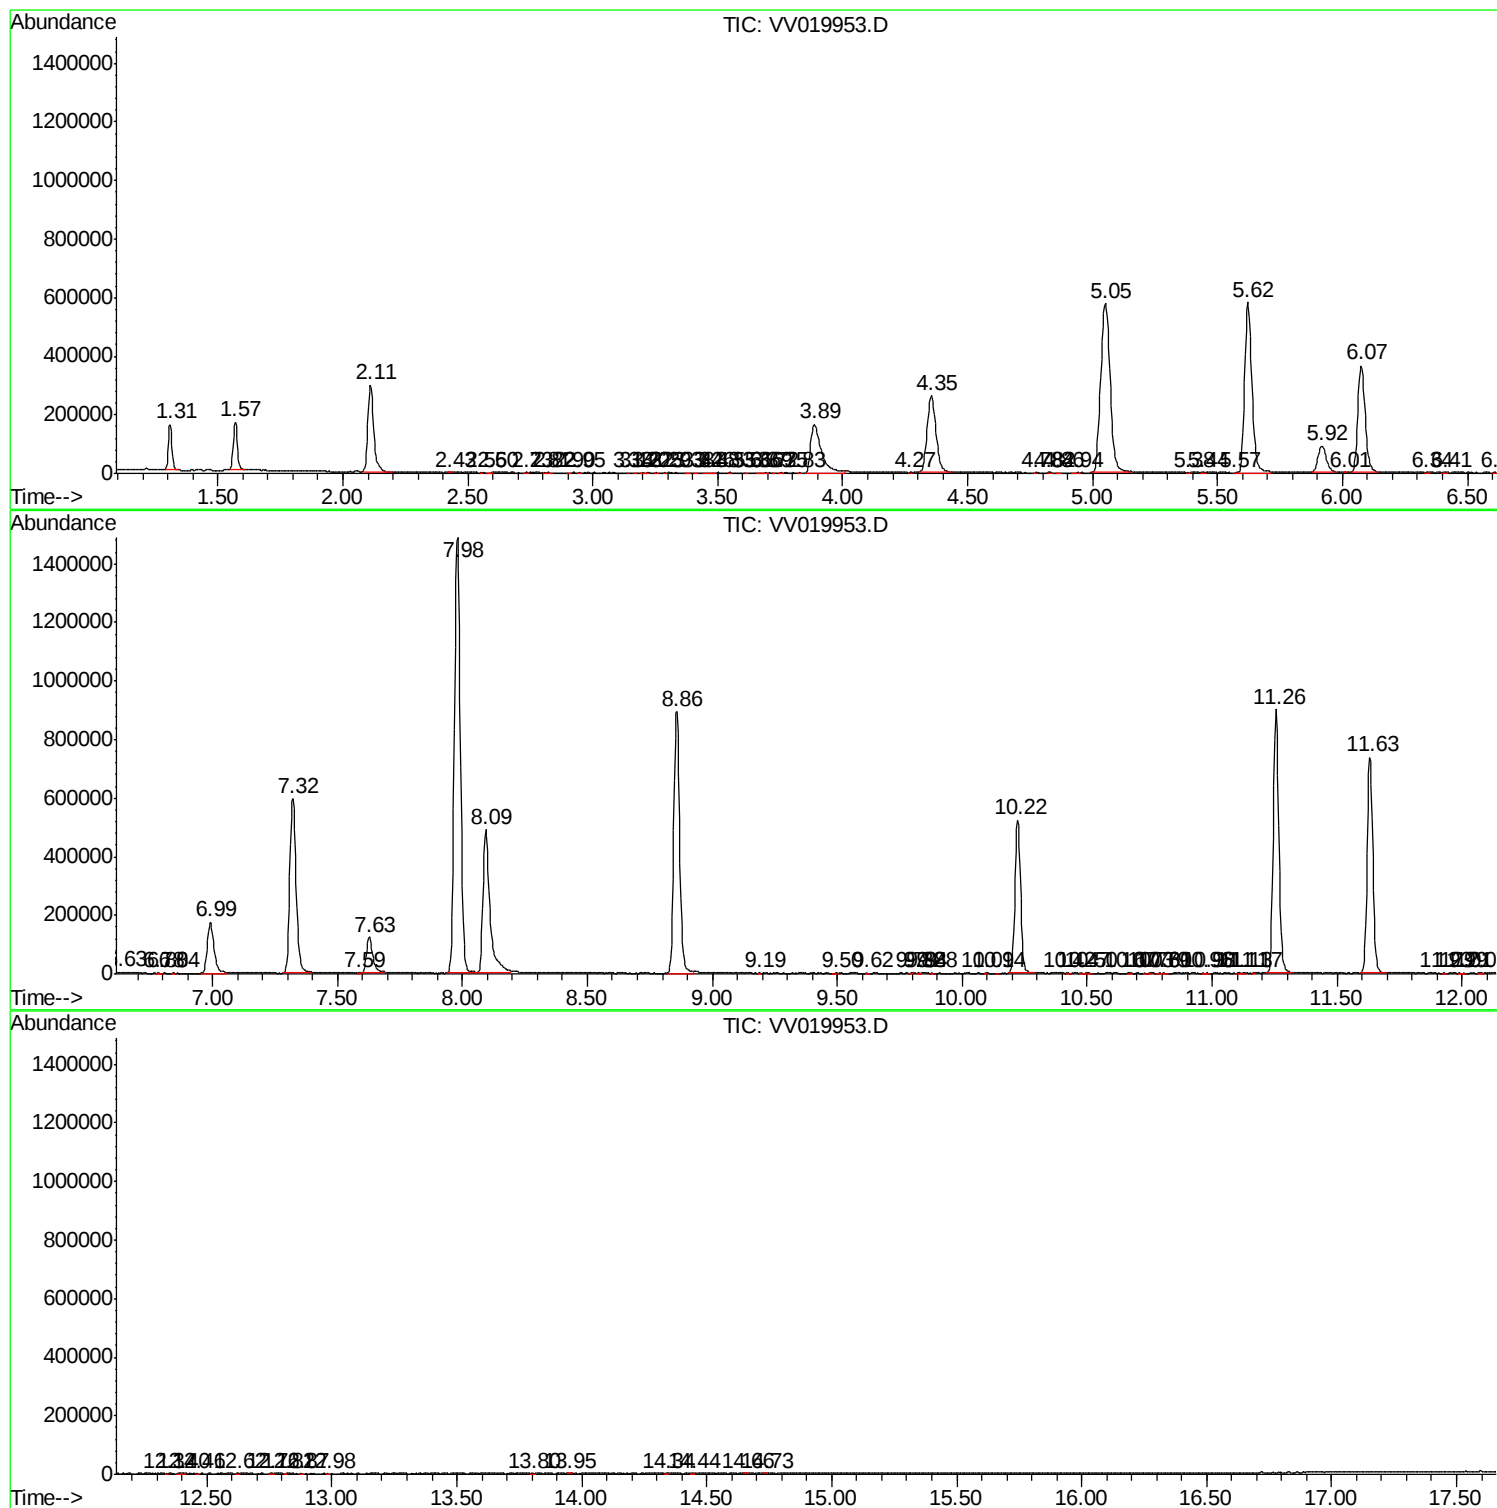

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019953.D
Acq On : 08 Jan 2021 17:34
Operator : SY/MD
Sample : M1064-03DL 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010821\
Data File : VV019953.D
Acq On : 08 Jan 2021 17:34
Operator : SY/MD
Sample : M1064-03DL 250X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4X4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc