

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019954.D
 Acq On : 08 Jan 2021 17:58
 Operator : SY/MD
 Sample : M1064-02DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	78	rVB	161943	156433	5.03%	0.978%
2	1.569	143	149	159	rVB	164475	177066	5.69%	1.107%
3	2.110	308	317	344	rVB	299462	482533	15.51%	3.017%
4	2.621	469	476	478	rBV8	1548	1794	0.06%	0.011%
5	2.772	521	523	529	rVB7	1374	993	0.03%	0.006%
6	2.807	531	534	537	rBV3	691	492	0.02%	0.003%
7	2.823	537	539	541	rBV2	606	382	0.01%	0.002%
8	2.859	548	550	555	rVB3	1086	618	0.02%	0.004%
9	2.926	569	571	574	rVB2	760	470	0.02%	0.003%
10	2.971	582	585	588	rBV4	1193	838	0.03%	0.005%
11	3.023	599	601	602	rBV2	795	365	0.01%	0.002%
12	3.122	630	632	640	rVB7	1422	1233	0.04%	0.008%
13	3.155	640	642	644	rBV2	825	400	0.01%	0.003%
14	3.251	668	672	674	rBV4	1105	972	0.03%	0.006%
15	3.280	678	681	684	rBV4	517	360	0.01%	0.002%
16	3.322	692	694	699	rVB4	764	622	0.02%	0.004%
17	3.351	699	703	705	rBV4	657	547	0.02%	0.003%
18	3.383	711	713	718	rBV3	890	618	0.02%	0.004%
19	3.457	733	736	737	rBV2	900	364	0.01%	0.002%
20	3.508	750	752	756	rBV3	914	561	0.02%	0.004%
21	3.550	761	765	767	rVV4	601	439	0.01%	0.003%
22	3.634	788	791	794	rVV3	832	444	0.01%	0.003%
23	3.794	839	841	845	rVB3	618	376	0.01%	0.002%
24	3.888	859	870	901	rBV	163399	483740	15.55%	3.024%
25	4.354	1000	1015	1043	rBV	258830	645597	20.75%	4.036%
26	4.515	1063	1065	1066	rBV	1005	482	0.02%	0.003%
27	4.659	1106	1110	1112	rBV3	1030	563	0.02%	0.004%
28	4.672	1112	1114	1116	rBV2	854	423	0.01%	0.003%
29	4.724	1127	1130	1132	rVB3	929	440	0.01%	0.003%
30	4.762	1141	1142	1147	rVB4	1071	612	0.02%	0.004%
31	4.785	1147	1149	1152	rBV4	757	462	0.01%	0.003%
32	4.900	1180	1185	1188	rBV4	939	840	0.03%	0.005%
33	4.984	1205	1211	1213	rBV7	861	926	0.03%	0.006%
34	5.052	1215	1232	1260	rBV2	578970	1514973	48.70%	9.471%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019954.D
 Acq On : 08 Jan 2021 17:58
 Operator : SY/MD
 Sample : M1064-02DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	5.331	1317	1319	1321	rBV5	925	458	0.01%	0.003%
36	5.621	1396	1409	1443	rBV	555921	1126178	36.20%	7.041%
37	5.916	1490	1501	1519	rVB4	102884	233784	7.51%	1.462%
38	6.074	1538	1550	1577	rVB2	365137	737290	23.70%	4.609%
39	6.341	1629	1633	1635	rBV4	1359	946	0.03%	0.006%
40	6.425	1653	1659	1661	rBV7	1006	950	0.03%	0.006%
41	6.582	1705	1708	1709	rBV2	831	427	0.01%	0.003%
42	6.598	1710	1713	1716	rVB3	1279	771	0.02%	0.005%
43	6.643	1718	1727	1735	rBV10	2112	4510	0.14%	0.028%
44	6.859	1791	1794	1797	rBV4	786	662	0.02%	0.004%
45	6.990	1823	1835	1858	rBV	178709	332393	10.68%	2.078%
46	7.135	1878	1880	1882	rBV3	1004	515	0.02%	0.003%
47	7.322	1926	1938	1962	rBV	606320	1059786	34.07%	6.626%
48	7.627	2023	2033	2057	rBV	121249	218879	7.04%	1.368%
49	7.913	2119	2122	2124	rBV2	876	668	0.02%	0.004%
50	7.981	2128	2143	2167	rBV	1851286	3110915	100.00%	19.449%
51	8.093	2169	2178	2211	rVV2	478391	933234	30.00%	5.834%
52	8.595	2331	2334	2336	rBV3	983	808	0.03%	0.005%
53	8.785	2391	2393	2396	rBV2	582	381	0.01%	0.002%
54	8.858	2403	2416	2436	rBV	852508	1397182	44.91%	8.735%
55	9.203	2521	2523	2525	rVB3	971	414	0.01%	0.003%
56	9.215	2525	2527	2530	rBV3	1107	848	0.03%	0.005%
57	9.334	2560	2564	2565	rBV2	1008	690	0.02%	0.004%
58	9.363	2571	2573	2575	rBV3	1030	413	0.01%	0.003%
59	9.511	2617	2619	2622	rBV	869	381	0.01%	0.002%
60	9.559	2631	2634	2636	rBV3	771	539	0.02%	0.003%
61	9.575	2637	2639	2641	rBV3	989	476	0.02%	0.003%
62	9.791	2704	2706	2711	rVB5	1297	783	0.03%	0.005%
63	9.813	2711	2713	2715	rBV2	807	460	0.01%	0.003%
64	9.826	2715	2717	2719	rBV3	1028	679	0.02%	0.004%
65	9.945	2750	2754	2757	rBV4	859	624	0.02%	0.004%
66	10.096	2797	2801	2802	rBV3	700	500	0.02%	0.003%
67	10.106	2802	2804	2809	rVV3	1030	675	0.02%	0.004%
68	10.138	2812	2814	2816	rVV2	1029	518	0.02%	0.003%
69	10.222	2829	2840	2859	rBV	514108	815128	26.20%	5.096%
70	10.373	2884	2887	2889	rBV2	951	717	0.02%	0.004%
71	10.392	2889	2893	2896	rVB4	1301	1128	0.04%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019954.D
 Acq On : 08 Jan 2021 17:58
 Operator : SY/MD
 Sample : M1064-02DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.408	2896	2898	2900	rBV4	1089	538	0.02%	0.003%
73	10.453	2910	2912	2914	rVB4	840	402	0.01%	0.003%
74	10.688	2981	2985	2987	rBV4	1133	751	0.02%	0.005%
75	10.746	2998	3003	3010	rVB6	1051	1298	0.04%	0.008%
76	11.000	3077	3082	3083	rBV3	1143	999	0.03%	0.006%
77	11.038	3089	3094	3096	rBV4	1377	959	0.03%	0.006%
78	11.109	3114	3116	3122	rVB4	1239	1115	0.04%	0.007%
79	11.135	3122	3124	3125	rBV	789	426	0.01%	0.003%
80	11.257	3150	3162	3186	rBV	847670	1341013	43.11%	8.384%
81	11.431	3214	3216	3218	rBV2	804	503	0.02%	0.003%
82	11.466	3224	3227	3229	rBV5	1256	541	0.02%	0.003%
83	11.495	3234	3236	3239	rBV3	731	383	0.01%	0.002%
84	11.518	3241	3243	3245	rBV2	880	537	0.02%	0.003%
85	11.630	3266	3278	3300	rBV	739878	1169579	37.60%	7.312%
86	11.981	3385	3387	3391	rVB4	1064	619	0.02%	0.004%
87	12.482	3540	3543	3546	rBV2	917	708	0.02%	0.004%
88	12.627	3586	3588	3593	rBV5	1132	1073	0.03%	0.007%
89	12.717	3614	3616	3622	rBV6	1135	1176	0.04%	0.007%
90	12.817	3645	3647	3653	rBV4	819	943	0.03%	0.006%
91	12.845	3653	3656	3658	rBV3	1201	844	0.03%	0.005%
92	12.932	3680	3683	3685	rBV3	1252	777	0.02%	0.005%
93	13.099	3731	3735	3736	rBV4	792	661	0.02%	0.004%
94	13.135	3743	3746	3749	rBV4	826	542	0.02%	0.003%
95	13.228	3773	3775	3781	rVB4	1357	969	0.03%	0.006%
96	13.749	3935	3937	3940	rBV2	1007	552	0.02%	0.003%
97	14.099	4044	4046	4050	rVB4	967	457	0.01%	0.003%
98	14.209	4077	4080	4086	rBV6	1565	1409	0.05%	0.009%
99	14.636	4210	4213	4215	rBV5	1185	863	0.03%	0.005%
100	15.238	4398	4400	4404	rVB4	1777	1033	0.03%	0.006%


Sum of corrected areas: 15995358

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010821\
Data File : VV019954.D
Acq On : 08 Jan 2021 17:58
Operator : SY/MD
Sample : M1064-02DL 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

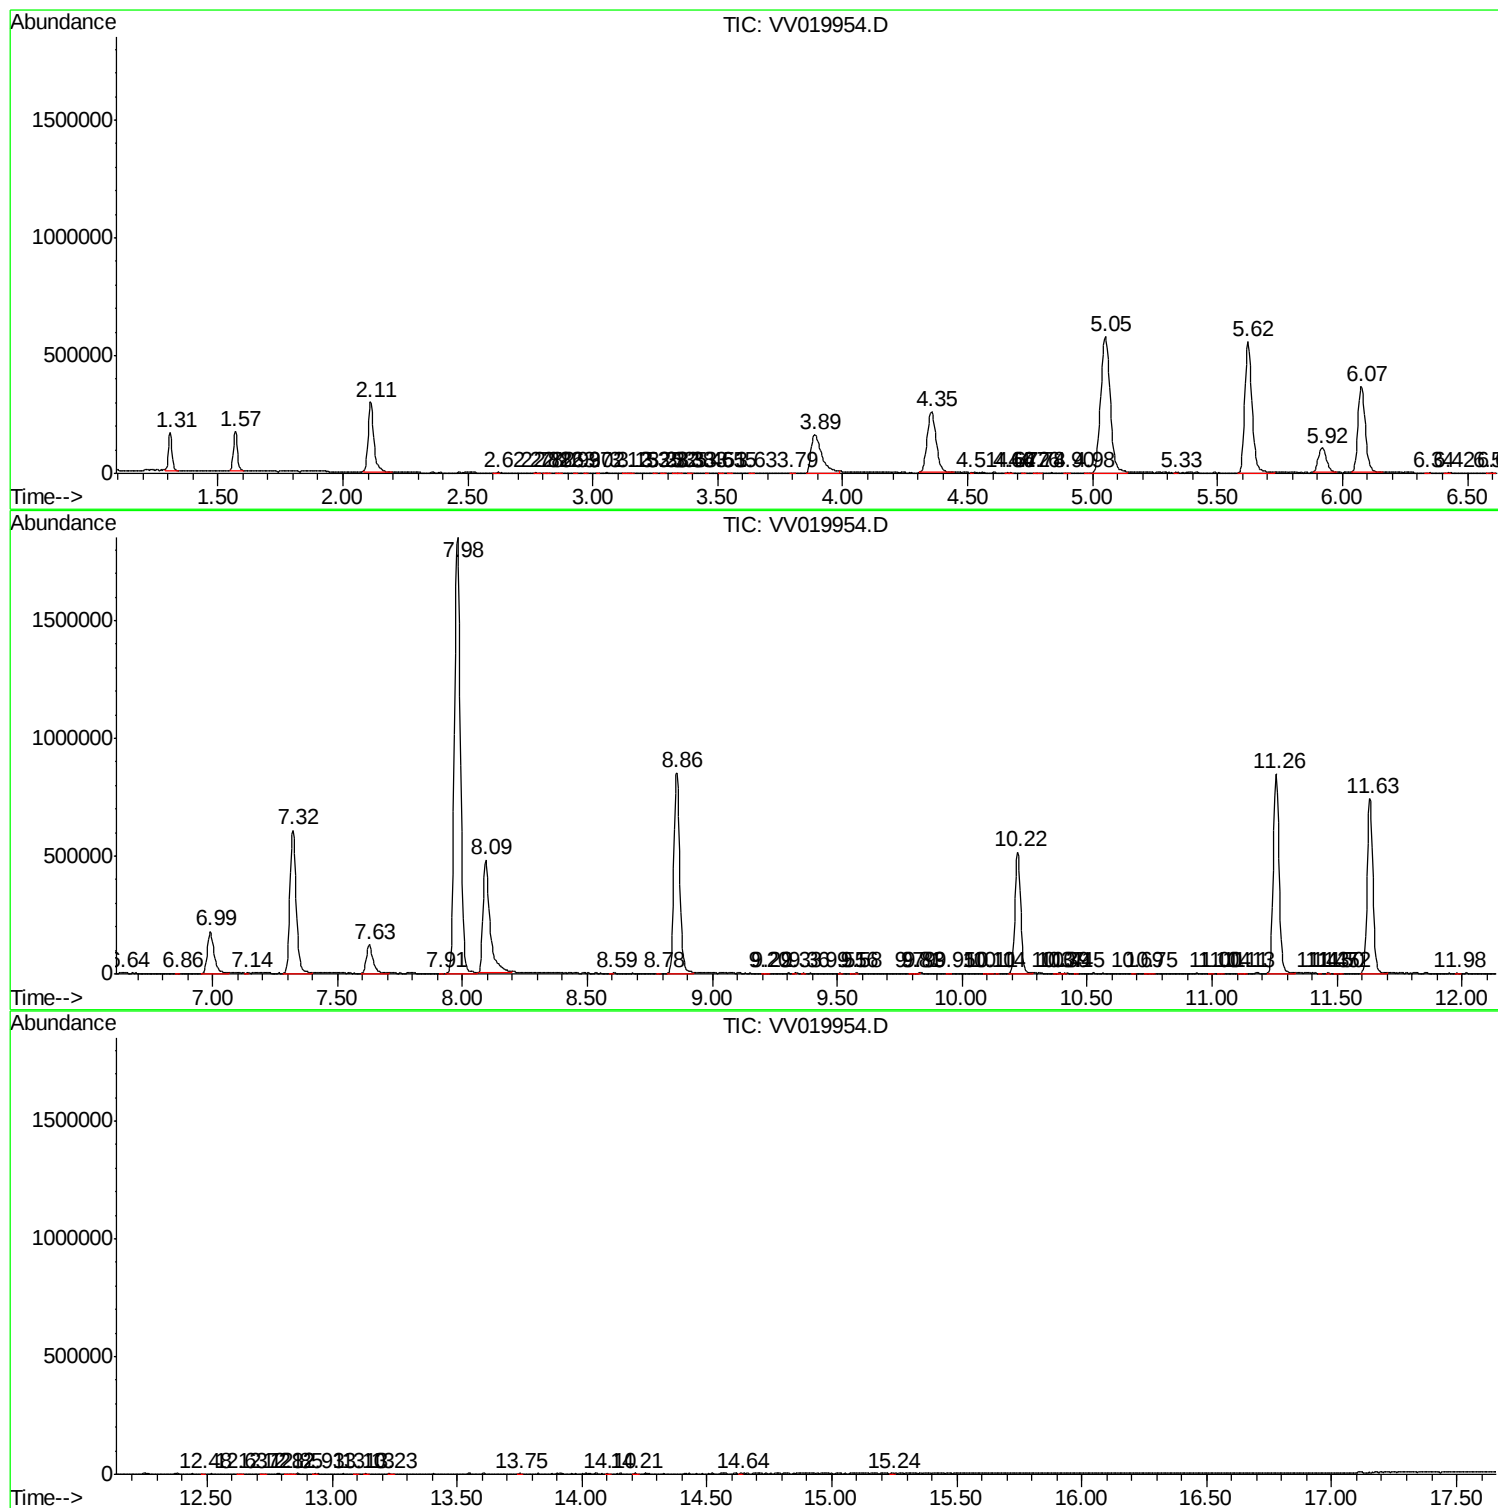

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019954.D
Acq On : 08 Jan 2021 17:58
Operator : SY/MD
Sample : M1064-02DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010821\
Data File : VV019954.D
Acq On : 08 Jan 2021 17:58
Operator : SY/MD
Sample : M1064-02DL 500X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4X3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc